

AS IV Serial no: 097419
Version no: 532B

TEST RECORD 00071

Temp Date Time ^{s/} 210L

Air Blank:
08/13/14 18:36 .000
Calibration Check:
23 08/13/14 18:36 .096

Subject Name
CALIBRATION CHECK
Subject I.D.

Operator Name, I.D.
Ronald C. Bay #501
Location
PACMIRA PD

AS IV Serial no: 097419
Version no: 532B

TEST RECORD 00072

Temp Date Time ^{s/} 210L

Air Blank:
08/13/14 18:37 .000
Calibration Check:
23 08/13/14 18:37 .096

Subject Name
CALIBRATION CHECK
Subject I.D.

Operator Name, I.D.
Ronald C. Bay #501
Location
PACMIRA PD

AS IV Serial no: 097419
Version no: 532B

TEST RECORD 00073

Temp Date Time ^{s/} 210L

Air Blank:
08/13/14 18:39 .000
Calibration Check:
24 08/13/14 18:39 .097

Subject Name
CALIBRATION CHECK
Subject I.D.

Operator Name, I.D.
Ronald C. Bay #501
Location
PACMIRA PD

AS IV Serial no: 097419
Version no: 532B

TEST RECORD 00074

Temp Date Time ^{s/} 210L

VOID: RFI
12 08/13/14 18:40

Subject Name
RFI TEST
Subject I.D.

Operator Name, I.D.
Ronald C. Bay #501
Location
PACMIRA PD



GUTH LABORATORIES, INC.

590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number **14110** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on **May 5, 2014**, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.1206%** (w/vol) ethyl alcohol. The expiration date for this lot number is **May 1, 2016** at 11:59 PM.

When used in a calibrated Simulator, operating at $34^{\circ}\text{C} \pm .2^{\circ}\text{C}$, this solution will give a breath alcohol analysis instrument reading of **0.100 g/210L** \pm 3%.


The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President
GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
RONALD C PEER

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 7/22/2014

NUMBER 240306

EXPIRES 7/22/2016

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO-909-0771 (6-10)

LAB-1 (06-10)



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.




Operator PEER, RONALD
 Permit No 240306
 Date Issued 7/22/2014 Date Expires 7/22/2016



Simulator Calibration Report

This calibration report is to certify the alcohol reference simulator listed below has been examined and tested using standards traceable to the National Institute of Standards and Technology (NIST) in accordance with the standards set by the Missouri Department of Health and Senior Services Rules and Regulations:
19 CSR 25-30.051 (4).

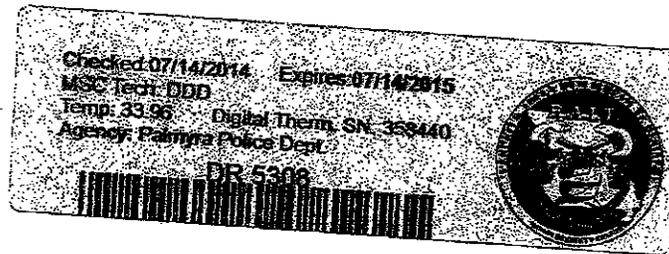

Technician Printed Name: DONALD D. DEBEARD

Technician Signature: Donald D. DeBeard

Date: 07/14/2014

Contact: Missouri Safety Center

Breath-Alcohol Instrument Training Program

660-543-4834