



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

REPORT #6

**RECEIVED**

By Carol Day at 12:44 pm, Apr 25, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 30 days). Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service. Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201191	NAME OF AGENCY .Claycomo.Police.Department	DATE OF INSPECTION .04/24/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 115 E. 69 Highway		TIME OF INSPECTION 10:06 am

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) <u>04/24/14 10:16</u>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER <u>49°C</u>	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

<input checked="" type="checkbox"/> INDICATOR LIGHTS
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER <u>RepCo marketing</u> LOT # <u>13002</u> EXP. DATE <u>06/19/2015</u>
<input checked="" type="checkbox"/> SIMULATOR TEMP ( $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$ ) <u>34.0</u> °C SIMULATOR SN <u>SD1353</u> EXP. DATE <u>02/27/2015</u>

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within  $\pm 5\%$  of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 $\blackleftarrow$ .102	TEST 2 $\blackleftarrow$ .102	TEST 3 $\blackleftarrow$ .102
-------------------------------	-------------------------------	-------------------------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	1	(.0-.04)	0	(.05-.09)	1	(.10-.14)	0	(.15-.19)	0	OVER .19	0
----------	---	----------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).  
 Operates within D.H.S.S. standards

<b>INSPECTING OFFICER</b>	
SIGNATURE 	PRINT FULL NAME Matthew E. Beets
TYPE II PERMIT NUMBER/EXPIRATION DATE 220401 12/20/14	TELEPHONE NUMBER (816) 452-4613

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
 2875 James Blvd.  
 Poplar Bluff, MO 63901

**CERTIFICATE OF ANALYSIS**

**MANUFACTURER AND SUPPLIER:** RepCo Marketing, Inc.

**LOT NUMBER:** 13002

**EXPIRATION DATE:** June 19, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013  
The expiration date for this lot number is June 19, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President  
RepCo Marketing, Inc.

# BAC DataMaster Evidence Ticket

STATE OF MICHIGAN  
CLEVELAND POLICE DEPARTMENT

THE ASSIGNED SERIAL NUMBER IS: 10126  
10126

--- DIAGNOSTIC CHECK ---

COMPUTER:	ONLY
PROGRAM (91-97-9999):	ONLY
MEASURES	
SAMPLE NUMBER:	000
FLAM DETECTOR:	ONLY
PUMP	
HIGH SPEED:	ONLY
DETECTION:	ONLY
FILTERS:	ONLY
SUBSTRATE SAMPLES:	ONLY
CALIBRATION:	ONLY

PREVIOUS TEST:

PREVIOUS TEST RESULTS: 10126  
10126

Operator Signature



2208-02

# BAC DataMaster Evidence Ticket

STATE OF MICHIGAN  
CLEVELAND POLICE DEPARTMENT

THE ASSIGNED SERIAL NUMBER IS: 10126  
10126

ORIGIN TYPE: ONLY

SUBJECT NUMBER:

REF/YES

BODY AS SAMPLE: ONLY

STATE/DIVISION: ONLY

ARRESTING OFFICER:

SECTS/ARTICLE:

CENTERS I.D. ONLY

TESTING BY CODE:

REFS: ONLY

OFFICER I.D. ONLY

OFFICER: ONLY

EMPLOYER: ONLY

WSP/LEAD: ONLY

REFI TEST: ONLY

--- PREVIOUS TESTS ---

BLANK TEST	000	10126
INTERNAL STANDARD	VERIFIED	10126
RADIO INTERFERENCE		

Operator Signature



2208-01

Face This Side Down - This Edge In First

# BAC DataMaster Evidence Ticket

STATE OF MISSISSIPPI  
DEPARTMENT OF TRANSPORTATION

OFFICE OF MOTOR VEHICLE SAFETY, MONROE, LOUISIANA  
B-4-10-10

VEHICLE OFFICER:  
RESPONSIBILITY  
OFFENSE VIOLATION  
PERMIT CLASSIFICATION  
EXPIRATION DATE  
MISCELLANEOUS NOTES  
MONTHLY PERCENTAGE

--- REFERENCE ---

BLANK TEST	1.10	19119
INTERNAL STANDARD	1.10	19119
EXTERNAL STANDARD	1.10	19119
BLANK TEST	1.10	19119
INTERNAL STANDARD	1.10	19119
EXTERNAL STANDARD	1.10	19119
BLANK TEST	1.10	19119

R = 0  
S.D. = 0.1  
S.V. = 0.02

Operator Signature



State of Missouri  
DEPARTMENT OF HEALTH



P E R M I T  
TYPE II



MATTHEW E BEETS

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

Date 12/20/2012

Number 220401

Expires 12/20/2014

MO 580-0771 (7-88)

Director of State Public Health Laboratory

ACTING DIRECTOR

Director, Department of Health

Lab. 4 (R7-88)




## Simulator Calibration Report

This calibration report is to certify the alcohol reference simulator listed below has been examined and tested using standards traceable to the National Institute of Standards and Technology (NIST) in accordance with the standards set by the Missouri Department of Health and Senior Services Rules and Regulations: 19 CSR 25-30.051 (4).

Checked: 2/27/2014 Expires: 02/27/2015  
Digital Therm. SN:094948 Temp:33.98  
MSC Tech:DRL  
Agency: Claycomo Police Department  
SD1353



Technician Printed Name: Dan Lucas

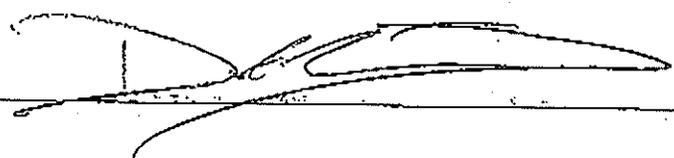Technician Signature: 

Date: 02/27/2014

Contact: Missouri Safety Center

Breath-Alcohol Instrument Training Program

660-543-4834