

MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED
 By Carol Day at 2:04 pm, Nov 17, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201191	NAME OF AGENCY Claycomo P.D.	DATE OF INSPECTION 11/14/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 115 E. 69 Hwy. Claycomo		TIME OF INSPECTION 9:34 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 11/14/14 0934
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER _____ 49°C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER RepCo Marketing LOT # 13002 EXP. DATE 06/19/2015

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN SD1353 EXP. DATE 02/27/2015

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

- 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
- 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
- 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1	TEST 2	TEST 3
--------	--------	--------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	1	(0-.04)	(.05-.09)	(.10-.14)	(.15-.19)	1	OVER .19
----------	---	---------	-----------	-----------	-----------	---	----------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).
 Operates within D.H.S.S. standards

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME Matthew E. Beets
---------------	-------------------------------------

TYPE II PERMIT NUMBER/EXPIRATION DATE 220401 12/20/2014	TELEPHONE NUMBER (816) 452-4613
--	------------------------------------

RETURN COMPLETED REPORT TO THE:
 Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
 2875 James Blvd.
 Poplar Bluff, MO 63901

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.
LOT NUMBER: 13002
EXPIRATION DATE: June 19, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/-3% gms/210L Breath when heated to 34 Degrees Celsius +/-0.2 Degree Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013
The expiration date for this lot number is June 19, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.

BAC DataMaster
Evidence Ticket

OFFICE OF MISSOURI
UNIVERSITY POLICE DEPARTMENT

ANALYZER SERIAL NUMBER 391191
11/16/14
99134

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM (04-07-2009): OKAY
HEATERS
SAMPLE CHAMBER: 49c
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopq
rstuvwxyz{|}~*

Operator Signature



BAC DataMaster Evidence Ticket

STATE OF MISSISSIPPI
SHERIFFS POLICE DEPARTMENT

BAC DEPARTMENT SERIAL NUMBER 281191
11/14/14


TESTING OFFICER:
SEETS/MATTHEW/E
OFFICER I.D.# 119
PERMIT NUMBER: 280401
EXPIRATION DATE: 12/28/14
MISCELLANEOUS DATA:
MONTHLY PRINT/INTERMEDIATE

--- SUPERVISOR NAME ---

BLANK TEST	.000	09:39
INTERNAL STANDARD	VERIFIED	09:39
EXTERNAL STANDARD	.000	09:40
BLANK TEST	.000	09:40
EXTERNAL STANDARD	.000	09:41
BLANK TEST	.000	09:42
EXTERNAL STANDARD	.000	09:42
BLANK TEST	.000	09:43

N = 3
SIM. = .1
AVG. = .09%

Operator Signature



2208-02

BAC DataMaster Evidence Ticket

STATE OF MISSISSIPPI
SHERIFFS POLICE DEPARTMENT


BAC DEPARTMENT SERIAL NUMBER 281191
11/14/14

ARREST TIME: 09:00
SUBJECT NAME:
OFFICER:
DOB: 11/10/1981 SEX: M
STATE I.D.#: 1234567
TESTING OFFICER:
SEETS/MATTHEW/E
OFFICER I.D.#: 119
TESTING OFFICER:
SEETS/MATTHEW/E
OFFICER I.D.#: 119
PERMIT NUMBER: 280401
EXPIRATION DATE: 12/28/14
MISCELLANEOUS DATA:
RFI TEST MONTHLY PRINT.

--- BREATH ANALYSIS ---

BLANK TEST	.000	09:55
INTERNAL STANDARD	VERIFIED	09:55
RADIO INTERFERENCE		

Operator Signature



2208-02

DEPARTMENT OF HEALTH



PERMIT
TYPE II



MATTHEW E BEETS

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

Date 12/20/2012

Number 220401

Expires 12/20/2014

Director of State Public Health Laboratory

ACTING DIRECTOR

Director, Department of Health




Simulator Calibration Report

This calibration report is to certify the alcohol reference simulator listed below has been examined and tested using standards traceable to the National Institute of Standards and Technology (NIST) in accordance with the standards set by the Missouri Department of Health and Senior Services Rules and Regulations:
19 CSR 25-30.051 (4).

Checked: 2/27/2014 Expires: 02/27/2015
Digital Therm. SN:094948 Temp:33.98
MSC Tech:DRL
Agency: Claycomo Police Department
SD1353



Technician Printed Name: Dan Lucas

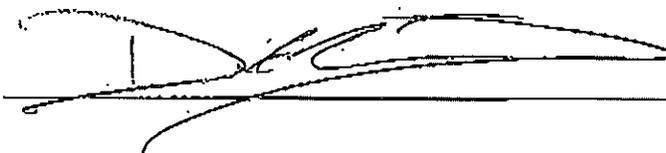Technician Signature: 

Date: 02/27/2014

Contact: Missouri Safety Center
Breath-Alcohol Instrument Training Program
660-543-4834