



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED 3/4/14-CD

REVIEWED REPORT #6
 By Carol Day at 9:56 am, Mar 14, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201241	NAME OF AGENCY TOWN AND COUNTRY POLICE DEPARTMENT	DATE OF INSPECTION 02/24/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 1011 MUNICIPAL CENTER DRIVE TOWN AND COUNTRY, MO. 63131		TIME OF INSPECTION 4:52 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) <u>02/24/2014 04:52</u>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER <u>49 °C</u>	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

<input checked="" type="checkbox"/> INDICATOR LIGHTS
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER <u>REPCO MARKETING INC</u> LOT # <u>13002</u> EXP. DATE <u>06/19/2015</u>
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) <u>34.0</u> °C SIMULATOR SN <u>SD2781</u> EXP. DATE <u>11/21/2014</u>

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 \blackhearts .096%	TEST 2 \blackhearts .097%	TEST 3 \blackhearts .097%
-----------------------------	-----------------------------	-----------------------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	7	(0-.04)	0	(.05-.09)	2	(.10-.14)	11	(.15-.19)	5	OVER .19	1
----------	---	---------	---	-----------	---	-----------	----	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

INSPECTING OFFICER	
SIGNATURE 	PRINT FULL NAME WM. CHRIS MOORE
TYPE II PERMIT NUMBER EXPIRATION DATE 220302 09/25/2014	TELEPHONE NUMBER (314) 432-4697

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
 2875 James Blvd.
 Poplar Bluff, MO 63901

REPCO MARKETING INC.

3101-188 STONYBROCK DRIVE
RALEIGH, N.C. 27604
919-876-5480

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.
LOT NUMBER: 13002
EXPIRATION DATE: June 19, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013
The expiration date for this lot number is June 19, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
TOWN AND COUNTRY POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201241
02/24/14


TESTING OFFICER:
MOORE/M/CHRIS
OFFICER I.D.# 83
PERMIT NUMBER: 28302
EXPIRATION DATE: 09/25/14
MISCELLANEOUS DATA:

--- SUPERVISOR NAME ---

BLANK TEST	.000	04:57
INTERNAL STANDARD	VERIFIED	04:57
EXTERNAL STANDARD	.006	04:57
BLANK TEST	.006	04:58
EXTERNAL STANDARD	.007	04:58
BLANK TEST	.006	04:59
EXTERNAL STANDARD	.007	04:59
BLANK TEST	.000	05:00

N = 3
SIM. = .1
AVG. = .0966

Operator Signature

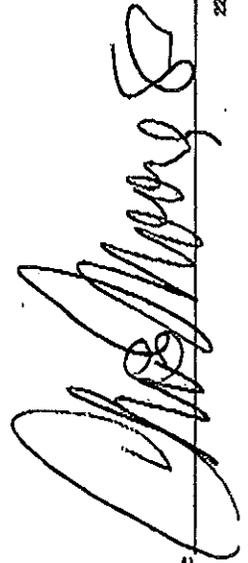

2208-02

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
TOWN AND COUNTRY POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201241
02/24/14
04:52

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM (04-07-2009): OKAY

HEATERS
SAMPLE CHAMBER: 49c

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY


DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
!@#%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUWXYZ[\]^_`abcde fghijklmnop
qrs tuvwxyz{|}~*

Operator Signature

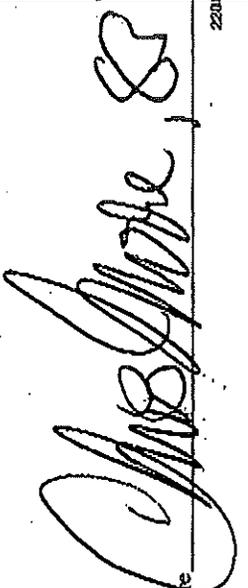

2208-0

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
TOWN AND COUNTRY POLICE DEPARTMENT


BAC DATAMASTER SERIAL NUMBER 281241
02/24/14

ARREST TIME: 04:00
SUBJECT NAME:
MOUSE/MIGHTY
DOB: 12/12/12 SEX: M
STATE/D.L.: FL/123456789
ARRESTING OFFICER:
MOORE/M/CHRIS
OFFICER I.D.: 83
TESTING OFFICER:
MOORE/M/CHRIS
OFFICER I.D.: 83
PERMIT NUMBER: 22002
EXPIRATION DATE: 09/25/14
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST .000 05:02
INTERNAL STANDARD VERIFIED 05:02
RADIO INTERFERENCE

Operator Signature

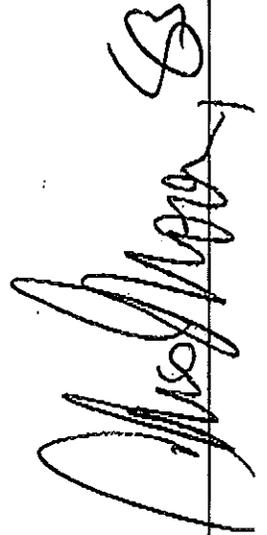

State of Missouri
DEPARTMENT OF HEALTH



P E R M I T
TYPE II



WILLIAM C MOORE

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

Date 09/25/2012

Number 220302

Expires 09/25/2014

Director of State Public Health Laboratory

Director, Department of Health