



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED REPORT #6
 By Carol Day at 1:49 pm, Apr 23, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201243	NAME OF AGENCY West Plains Police Department	DATE OF INSPECTION 04/21/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 1912 Holiday Lane, West Plains		TIME OF INSPECTION 5:42 pm

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 04/21/2014 1742
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

<input checked="" type="checkbox"/> INDICATOR LIGHTS
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER Repco LOT # 13002 EXP. DATE 06/19/2015
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN DR6928 EXP. DATE 07/10/2014

CALIBRATION CHECK – (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 • .099	TEST 2 • .100	TEST 3 • .101
---------------	---------------	---------------

PERFORM B.F.I. TEST (PRINTOUT ATTACHED)

**INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF ADMINISTERED TESTS)**

REFUSALS	0	(0-.04)	0	(.05-.09)	2	(.10-.14)	1	(.15-.19)	3	OVER .19	1
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

N/A

INSPECTING OFFICER	
SIGNATURE	PRINT FULL NAME Brandon Romans
TYPE II PERMIT NUMBER/EXPIRATION DATE 230066 04/23/2015	TELEPHONE NUMBER (417) 256-2244

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
 2875 James Blvd.
 Poplar Bluff, MO 63901

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.

LOT NUMBER: 13002

EXPIRATION DATE: June 19, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.


This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013
The expiration date for this lot number is June 19, 2015 at 11:59 p.m.


This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM



**PERMIT
TYPE II**

BRANDON ROMANS

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 04/23/2013

NUMBER 230066

EXPIRES 04/23/2015

W. S. ...

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

Darl Vosterly

Acting Director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)

MO 580-0771 (6-10)

Face This Side Down , This Edge In First

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
WEST PLAINS POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER PA1243
04/21/14
17:42


--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM (04-07-2009): OKAY
HEATERS
SAMPLE CHAMBER: 49F
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHI
HIJKL MNOPQRSTUVWXYZ[\]^_`abcdefghijklmnop
qrstuvwxyz{|}~

Operator Signature

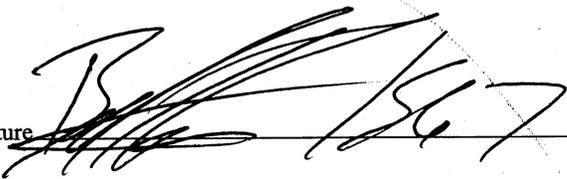

Face This Side Down - This Edge In First

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
WEST PLAINS POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER PA1243
04/21/14

TESTING OFFICER:
ROMANS/BRANDON
OFFICER I.D.: 567
PERMIT NUMBER: 230066
EXPIRATION DATE: 04/23/15
MISCELLANEOUS DATA:

--- SUPERVISOR NOTE ---

BLANK TEST	.000	17:44
INTERNAL STANDARD	VERIFIED	17:45
EXTERNAL STANDARD	.000	17:45
BLANK TEST	.000	17:46
EXTERNAL STANDARD	.100	17:46
BLANK TEST	.000	17:47
EXTERNAL STANDARD	.101	17:47
BLANK TEST	.000	17:48

N = 3
STM. = .1
AVG. = .1

Operator Signature



Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
WEST PLAINS POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER PA1P43
04/21/14

ARREST TIME: 16:30
SUBJECT NAME:
RFI/TEST
DOB: 09/09/89 SEX: M
STATE/D.L.I.: MO/767666
ARRESTING OFFICER:
ROMANS/BRANTON
OFFICER I.D.: 567
TESTING OFFICER:
ROMANS/BRANTON
OFFICER I.D.: 567
PERMIT NUMBER: 230066
EXPIRATION DATE: 04/23/15
MISCELLANEOUS DATA:
RFI TEST

--- BREATH ANALYSIS ---

BLANK TEST	.000	18:23
INTERNAL STANDARD	VERIFIED	18:23
RADIO INTERFERENCE		

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
WEST PLAINS POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER PA1P43
04/21/14

ARREST TIME: 16:30
SUBJECT NAME:
TEST
DOB: 09/09/89 SEX: M
STATE/D.L.I.: MO/767666
ARRESTING OFFICER:
ROMANS/BRANTON
OFFICER I.D.: 567
TESTING OFFICER:
ROMANS/BRANTON
OFFICER I.D.: 567
PERMIT NUMBER: 230066
EXPIRATION DATE: 04/23/15
MISCELLANEOUS DATA:
TEST

--- BREATH ANALYSIS ---

BLANK TEST	.000	18:25
INTERNAL STANDARD	VERIFIED	18:25
SUBJECT SAMPLE	.000	18:25
BLANK TEST	.000	18:26

4 seconds

Operator Signature 

Operator Signature 