



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

**RECEIVED**  
 By Carol Day at 1:15 pm, May 22, 2014

REPORT # 5

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201243	NAME OF AGENCY West Plains Police Department	DATE OF INSPECTION 05/22/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 1912 Holiday Lane, West Plains		TIME OF INSPECTION 8:54 am

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 05/22/2014 08:54
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER _____ 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Repro LOT # 13002 EXP. DATE 06/19/2015

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN DR6928 EXP. DATE 07/10/2014

CALIBRATION CHECK – (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

- 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1  .099	TEST 2  .100	TEST 3  .099
--------------	--------------	--------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

**INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)**

REFUSALS	0	(0-.04)	1	(.05-.09)	2	(.10-.14)	1	(.15-.19)	1	OVER .19	2
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

N/A

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME Brandon Romans
---------------	-----------------------------------

TYPE II PERMIT NUMBER/EXPIRATION DATE 230066 04/23/2015	TELEPHONE NUMBER (417) 256-2244
--	------------------------------------

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
 2875 James Blvd.  
 Poplar Bluff, MO 63901

**CERTIFICATE OF ANALYSIS**

**MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.**

**LOT NUMBER: 13002**

**EXPIRATION DATE: June 19, 2015 at 11:59 p.m.**

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013  
The expiration date for this lot number is June 19, 2015 at  
11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President  
RepCo Marketing, Inc.



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

2

**PERMIT  
TYPE II**

**BRANDON ROMANS**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 04/23/2013  
NUMBER 230066  
EXPIRES 04/23/2015

*W. S. R.*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Darl Voshell*

Acting Director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)

Face This Side Down - This Edge In First

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
WEST PLAINS POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 281243  
05/22/14  
08154

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM (04-07-0000): OKAY

HEATERS:  
SAMPLE CHAMBER: 49-

FILM DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!#\$%&'()\*+,-./:;<=>?@ABCDEFGHIJKL  
MNO PQRSTU VWXYZ[\]^\_`ab|cdefghijklmnop  
qrstuvwxyz{|}~

Operator Signature



Face This Side Down - This Edge In First

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
WEST PLAINS POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 281243  
05/22/14

TESTING OFFICER:

ROMANS/BRANDON

OFFICER I.D. #: 567

PERMIT NUMBER: 230066

EXPIRATION DATE: 04/23/15

MISSOURI ANALYSIS DATA:

--- SUPERVISOR NOTE ---


RI ANK TEST	.000	08:56
INTERNAL STANDARD	VERIFIED	08:56
EXTERNAL STANDARD	.000	08:57
RI ANK TEST	.000	08:58
EXTERNAL STANDARD	.100	08:58
RI ANK TEST	.000	08:59
EXTERNAL STANDARD	.000	08:59
RI ANK TEST	.000	09:00

N = 3

STDEV. = .1

AVG. = .0003

Operator Signature

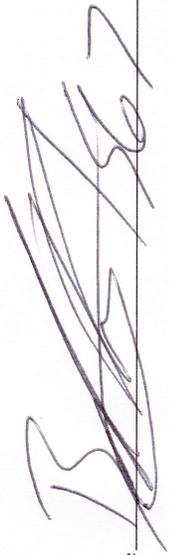

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
WEST PLAINS POLICE DEPARTMENT  
BAC DATAMASTER SERIAL NUMBER 201243  
05/22/14

ARREST TIME: 09:00  
SUBJECT NAME:  
REF TEST  
DOB: 09/09/99 SEX: M  
STATE/I.D.: MO/09090909  
ARRESTING OFFICER:  
ROMANS/BRANDON  
OFFICER I.D.: 567  
TESTING OFFICER:  
ROMANS/BRANDON  
OFFICER I.D.: 567  
PERMIT NUMBER: 200066  
EXPIRATION DATE: 04/23/15  
MISCELLANEOUS DATA:  
REF TEST

--- BREATH ANALYSIS ---  
RI BAK TEST .000 09:00  
INTERNAL STANDARD VERIFIED 09:00  
RABBIT INTERFERENCE

*[Handwritten Signature]*  
Operator Signature

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
WEST PLAINS POLICE DEPARTMENT  
BAC DATAMASTER SERIAL NUMBER 201243  
05/22/14

ARREST TIME: 09:00  
SUBJECT NAME:  
TEST  
DOB: 09/09/99 SEX: M  
STATE/I.D.: MO/09090909  
ARRESTING OFFICER:  
ROMANS/BRANDON  
OFFICER I.D.: 567  
TESTING OFFICER:  
ROMANS/BRANDON  
OFFICER I.D.: 567  
PERMIT NUMBER: 200066  
EXPIRATION DATE: 04/23/15  
MISCELLANEOUS DATA:  
TEST

--- BREATH ANALYSIS ---  
RI BAK TEST .000 09:05  
INTERNAL STANDARD VERIFIED 09:05  
SUBJECT SAMPLE .000 09:06  
RI BAK TEST .000 09:06

*4 Seconds*

*[Handwritten Signature]*  
Operator Signature