



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED
 By Carol Day at 3:10 pm, Jun 05, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATA MASTER SN 201252	NAME OF AGENCY Vinita Park Police Department	DATE OF INSPECTION 05/31/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 8374 Midland Blvd, Vinita Park, MO 63114		TIME OF INSPECTION 9:46 pm

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME: (from printout) <u>05/31/2014, 21:46</u>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER <u>34</u> °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

<input checked="" type="checkbox"/> INDICATOR LIGHTS
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER <u>Guth Laboratories</u> LOT # <u>12170</u> EXP. DATE <u>09/05/2014</u>
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) <u>34</u> °C SIMULATOR SN <u>SD2308</u> EXP. DATE <u>02/12/2015</u>

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 <u>.095</u>	TEST 2 <u>.097</u>	TEST 3 <u>.097</u>
--------------------	--------------------	--------------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	(0-.04)	(.05-.09)	(.10-.14)	(.15-.19)	OVER .19
----------	---------	-----------	-----------	-----------	----------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

Check Point 5-31-14

INSPECTING OFFICER	PRINT FULL NAME
SIGNATURE 	A. Klosterman DSN: 239
TYPE II PERMIT NUMBER/EXPIRATION DATE 230210, 10/02/2015	TELEPHONE NUMBER (314) 428-7373

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
 2875 James Blvd.
 Poplar Bluff, MO 63901



GUTH LABORATORIES, INC.

80 NORTH 6TH STREET • HARRISBURG, PA 17111-4811 • TELEPHONE: 717-634-6670

CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 12170 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on September 11, 2012, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1215% (w/vol) ethyl alcohol. The expiration date for this lot number is September 5, 2014 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President
GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201252
05/31/14

TESTING OFFICER:
KLOSTERMAN/ANDREW/J
OFFICER I.D.: 239
PERMIT NUMBER: 238210
EXPIRATION DATE: 10/02/15
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---

BLANK TEST	.000	21:42
INTERNAL STANDARD	VERIFIED	21:42
EXTERNAL STANDARD	.095	21:42
BLANK TEST	.000	21:43
EXTERNAL STANDARD	.097	21:43
BLANK TEST	.000	21:44
EXTERNAL STANDARD	.087	21:44
BLANK TEST	.000	21:45

N = 3
SIM. = .1
AVG. = .0963

[Signature]
1039

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201252
05/31/14
21:46

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM (04-07-2009): OKAY

HEATERS
SAMPLE CHAMBER: 49C

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~

[Signature]
1257

Face This Side Down - This Edge In First *ck 6, f*

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201252
05/31/14

ARREST TIME: 20:00
SUBJECT NAME:

RFI/CHECK
DOB: 05/31/14 SEX: M

STATE/D.L.: NR/NR
ARRESTING OFFICER:
NR

OFFICER I.D.: NH
TESTING OFFICER:

CLASSIFICATION NUMBER:
OFFICER I.D.: 239


PERMIT NUMBER: 230210
EXPIRATION DATE: 10/02/15

MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST	000	21:49
INTERNAL STANDARD	VERIFIED	
PRD10 INTERFERENCE		21:49

Operator Signature

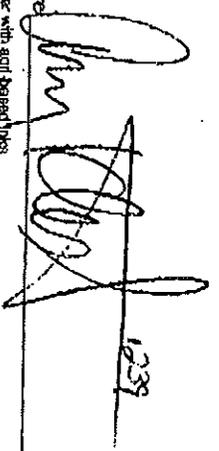

Printed on recycled paper with agri-based inks



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II

ANDREW KLOSTERMAN

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.


DATE 10/2/2013

NUMBER 230210

EXPIRES 10/2/2015

MO 680-0771 (6-10)


DIRECTOR OF STATE PUBLIC HEALTH LABORATORY


acting director
DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (05-10)

 STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator KLOSTERMAN, ANDREW
Permit No 230210
Date issued 10/2/2013 Date Expires 10/2/2015