

STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM  
DATAMASTER MAINTENANCE REPORT

RECEIVED 3/14/14-CD  
REPORT #6

REVIEWED  
By Carol Day at 9:37 am, Mar 14, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN: 201259  
NAME OF AGENCY: Boonville Police Department  
DATE OF INSPECTION: 03/06/2014

LOCATION OF INSTRUMENT (STREET AND CITY): 401 E. Morgan Street, Boonville MO 65233  
TIME OF INSPECTION: 03:44

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

DIAGNOSTIC CHECK (PRINTOUT ATTACHED) DATE AND TIME (from printout) 03:44  
 COMPUTER  DETECTOR  
 PROGRAM  FILTERS  
 HEATERS SAMPLE CHAMBER 48 °C  QUARTZ STANDARD  
 FLOW DETECTOR  CALIBRATION  
 PUMP HIGH SPEED  PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Guth Labs LOT # 13280 EXP. DATE 10/18/2013

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN SD3501 EXP. DATE 07/12/2013

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)  
Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)  
 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 = .096 TEST 2 = .097 TEST 3 = .097

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS 3 (0-.04) 1 (.05-.09) 0 (.10-.14) 0 (.15-.19) 0 OVER .19 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

INSPECTING OFFICER

SIGNATURE: [Signature] PRINT FULL NAME: James Décard  
TYPE II PERMIT NUMBER/EXPIRATION DATE: 220215 09/04/2014 TELEPHONE NUMBER: (660) 882-2727

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
2875 James Blvd.  
Poplar Bluff, MO 63901

**GUTH LABORATORIES, INC.**

690 NORTH 6TH STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-664-5470

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 13280 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on October 18, 2013, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1217% (w/vol) ethyl alcohol. The expiration date for this lot number is October 16, 2015 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
GUTH LABORATORIES, INC.

***NIST Traceability:***

*Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.*

*All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.*

PCAO DataMaster  
Evidence Tracker

STATE OF MISSOURI  
BOONVILLE POLICE DEPARTMENT  
BOONVILLE  
BAC/DWI REGISTER SERIAL NUMBER 201259  
03/06/14

ARREST TIME: 01:00  
SUBJECT NAME:

DOB: 01/01/80 SEX: F  
STATE/D.L.: KY/00000000  
ARRESTING OFFICER:

TESTING OFFICER:  
DECKARD/JAMES/M

OFFICER I.D.: 07  
PERMIT NUMBER: 220215

EXPIRATION DATE: 03/04/14  
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST .000 03:43  
INTERNAL STANDARD VERIFIED 03:43  
RADIO INTERFERENCE

Officer Signature



**BAE DataMaster**  
Evidence Tracker

STATE OF MISSOURI  
POLICE DEPARTMENT

BAE DATAMASTER SERIAL NUMBER 201239

03/06/14  
03:44

DIAGNOSTIC CHECK

COMPUTER: OKAY

PROGRAM (04-07-2009): OKAY

HEATERS  
SAMPLE CHAMBER: 48C

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY


CALIBRATION: OKAY

PRINTER TEST

! "#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~

Operator Signature



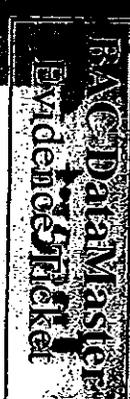

STATE OF MISSOURI  
BOONVILLE POLICE DEPARTMENT

BAC DRINKMASTER SERIAL NUMBER 201259  
03/06/14

TESTING OFFICER:  
DECKARD/JAMES/M  
OFFICER I.D.: 07  
PERMIT NUMBER: 220215  
EXPIRATION DATE: 09/04/14  
MISCELLANEOUS DATA:

--- SUPERVISOR NOTE ---

BLANK TEST	.000	03:52
INTERNAL STANDARD	VERIFIED	03:52
EXTERNAL STANDARD	.096	03:52
BLANK TEST	.000	03:53
EXTERNAL STANDARD	.097	03:53
BLANK TEST	.000	03:54
EXTERNAL STANDARD	.097	03:54
BLANK TEST	.000	03:55

N = 3  
Stm, = .1  
RWS, = .0966

Operator Signature

State of Missouri  
DEPARTMENT OF HEALTH



P E R M I T  
TYPE II



JAMES DECKARD

Is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

Date 09/04/2012

Number 220215

Expires 09/04/2014

MO 680-0771 (7-88)

Director of State Public Health Laboratory

Director, Department of Health

Lab. 4 (R7-88)