

MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
 DATAMASTER MAINTENANCE REPORT

**RECEIVED**  
 By Carol Day at 9:40 am, Dec 19, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN <b>201286</b>	NAME OF AGENCY <b>Mtn Grove Police</b>	DATE OF INSPECTION <b>12-17-2014</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>102 E. STATE Mtn Grove</b>		TIME OF INSPECTION <b>1244</b>

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) <b>12-17-2014 1244</b>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER <b>49</b> °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER **Guth** LOT # **14030** EXP. DATE **01/20/16**

SIMULATOR TEMP (34°C ± 0.2°C) **34.0** °C SIMULATOR SN **SD3322** EXP. DATE **12-16-2015**

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1	TEST 2	TEST 3
--------	--------	--------

PERFORM F.L.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS (0-04) (05-09) (10-14) (15-19) OVER 19

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (SEE OTHER SIDE IF NECESSARY).

INSPECTING OFFICER	PRINT FULL NAME
SIGNATURE <b>Danny Bledsoe</b>	<b>Danny Bledsoe</b>
TYPE II PERMIT NUMBER/EXPIRATION DATE <b>240433 12-17-2016</b>	TELEPHONE NUMBER <b>417-926-5181</b>

RETURN COMPLETED REPORT TO THE:  
 Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
 2875 James Blvd.  
 Poplar Bluff, MO 63901



**GUTH LABORATORIES, INC.**

530 NORTH 6TH STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-554-5470

## CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 14030 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on January 22, 2014, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1215% (w/vol) ethyl alcohol. The expiration date for this lot number is January 20, 2016 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
GUTH LABORATORIES, INC.

***NIST Traceability:***

*Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.*

*All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.*

Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
MOUNTAIN GROVE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201286  
12/17/14

TESTING OFFICER:  
BLEDSOE/DANIEL  
OFFICER I.D.# 1261  
PERMIT NUMBER: 240433  
EXPIRATION DATE: 12/17/16  
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---

BLANK TEST	.000	12:56
INTERNAL STANDARD	VERIFIED	12:56
EXTERNAL STANDARD	.099	12:56
BLANK TEST	.000	12:57
EXTERNAL STANDARD	.099	12:57
BLANK TEST	.000	12:58
EXTERNAL STANDARD	.099	12:58
BLANK TEST	.000	12:59

N = 3  
SIA = .1  
AVS = .0986

Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
MOUNTAIN GROVE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201286  
12/17/14  
12:44

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM (04-07-2009):	OKAY
HEATERS	
SAMPLE CHAMBER:	49C
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()\*+,-./:0123456789:;[ \]^\_`@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstu  
vwxyz{|}~\*

*Daniel Bledsoe*

Operator Signature

*Daniel Bledsoe*

Operator Signature

Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
MOUNTAIN GROVE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201286  
12/17/14

ARREST TIME: 12:30  
SUBJECT NAME:  
RFI/TEST  
DOB: 01/01/01 SEX: M  
STATE/D.L.: MO/000000000  
ARRESTING OFFICER:  
BLEDSOE  
OFFICER I.D.: 1201  
TESTING OFFICER:  
BLEDSOE/DANIEL  
OFFICER I.D.: 1201  
PERMIT NUMBER: 240433  
EXPIRATION DATE: 12/17/16  
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST	.000	13:02
INTERNAL STANDARD	VERIFIED	13:02
RADIO INTERFERENCE		

Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
MOUNTAIN GROVE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201286  
12/17/14

ARREST TIME: 12:30  
SUBJECT NAME:  
RFI/TEST  
DOB: 01/01/01 SEX: M  
STATE/D.L.: MO/000000000  
ARRESTING OFFICER:  
BLEDSOE  
OFFICER I.D.: 1201  
TESTING OFFICER:  
BLEDSOE/DANIEL  
OFFICER I.D.: 1201  
PERMIT NUMBER: 240433  
EXPIRATION DATE: 12/17/16  
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---


BLANK TEST	.000	13:02
INTERNAL STANDARD	VERIFIED	13:02
SUBJECT SAMPLE	.000	13:02
BLANK TEST	.000	13:02

Operator Signature



2208-02

Operator Signature

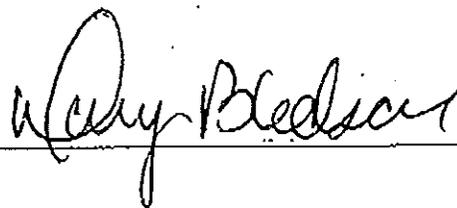



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



**PERMIT**  
 TYPE II

**DANIEL BLEDSOE**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER, INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 12/17/2014

NUMBER 240433

EXPIRES 12/17/2016

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Shad Vandenberg*

acting director  
 DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

40-280.0770 (8-13)

LAB-4 (95-10)