



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES

STATE PUBLIC HEALTH LABORATORY

BREATH ALCOHOL PROGRAM

DATAMASTER MAINTENANCE REPORT

RECEIVED 1/12/14-CD

REPORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days) whenever the instrument is serviced or repaired and whenever it is placed into service. Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

REVIEWED

By Carol Day at 8:54 am, Mar 14, 2014

DATAMASTER SN 201292	NAME OF AGENCY Owensville Police Dept	DATE OF INSPECTION 1-1-2014
LOCATION OF INSTRUMENT (STREET AND CITY) 109 N-2nd - Owensville, MO		TIME OF INSPECTION 0934

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 1-1-14 0934
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER
<input checked="" type="checkbox"/> INDICATOR LIGHTS	

<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER RepCo Marketing Inc	LOT # 13002	EXP. DATE 6-19-15
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) 34.0 C °C	SIMULATOR SN SD2300 094948	EXP. DATE 1-7-14

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 - .102	TEST 2 - .102	TEST 3 - .103
---------------	---------------	---------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT: (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS 2 (0-.04)	0 (.05-.09)	0 (.10-.14)	0 (.15-.19)	0 OVER .19
--------------------	-------------	-------------	-------------	------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).
Operating within DOT & Senior Service Standards

INSPECTING OFFICER	
SIGNATURE Robert Kicker	PRINT FULL NAME Robert Kicker
TYPE II PERMIT NUMBER/EXPIRATION DATE 220209 8-21-14	TELEPHONE NUMBER 573-437-2195
RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office 2875 James Blvd. Poplar Bluff, MO 63901	

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.

LOT NUMBER: 13002

EXPIRATION DATE: June 19, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).


The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013

The expiration date for this lot number is June 19, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.

Face This Side Down - This Edge In First

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
OWENSVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201292
01/01/14


TESTING OFFICER:
RICKERD/ROBERT
OFFICER I.D.: 101
PERMIT NUMBER: 220209
EXPIRATION DATE: 08/21/14
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---

BLANK TEST	.000	09:37
INTERNAL STANDARD	VERIFIED	09:37
EXTERNAL STANDARD	.102	09:38
BLANK TEST	.000	09:38
EXTERNAL STANDARD	.102	09:39
BLANK TEST	.000	09:39
EXTERNAL STANDARD	.103	09:39
BLANK TEST	.000	09:40

N = 3
SIM. = .1
AVG. = .1023

Operator Signature

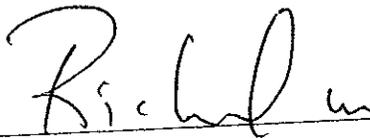

2208-02

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
OWENSVILLE POLICE DEPARTMENT

BAC DRTMMASTER SERIAL NUMBER 201292

01/01/14
09:34

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM (04-07-2009): OKAY
HERTERS
SAMPLE CHAMBER: 49C
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
!@#\$%^&*()~`-./0123456789:;<=>?ABBCDIEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde*fghijklmno
pqrstuvwxy{1}~`-`

Operator Signature



2208-02

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
OWENSVILLE POLICE DEPARTMENT

BAC DRTMMASTER SERIAL NUMBER 201292

01/01/14

ARREST TIME: 09:09
SUBJECT NAME:

WELK/TIM

DOB: 09/09/22 SEX: M

STATE/D.L.: MO/1111554

ARRESTING OFFICER:

RICKERD/ROBERT

OFFICER I.D.: 101

TESTING OFFICER:

RICKERD/ROBERT

OFFICER I.D.: 101

PERMIT NUMBER: 220209

EXPIRATION DATE: 08/21/14

MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST


.000 09:43

INTERNAL STANDARD

VERIFIED 09:43

RADIO INTERFERENCE

Operator Signature

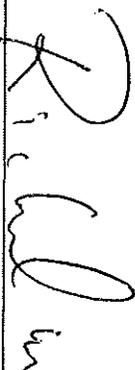

State of Missouri
DEPARTMENT OF HEALTH



P E R M I T
TYPE II



ROBERT RICKERD

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.041, RSMo 1986.

Date 08/21/2012

Number 220209

Expires 08/21/2014

MO 580-0771 (7-88)

W. S. W.

Director of State Public Health Laboratory

Maureen T. Donnelly

Director, Department of Health

Lab. 4 (R7-88)