



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

**RECEIVED** REPORT #6  
 By Carol Day at 2:08 pm, Feb 06, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 3 months).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN <u>201292</u>	NAME OF AGENCY <u>Owensville Police Dept.</u>	DATE OF INSPECTION <u>2-1-14</u>
LOCATION OF INSTRUMENT (STREET AND CITY) <u>109 N-2nd St Owensville-MO</u>		TIME OF INSPECTION <u>0632</u>

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) <u>2-1-14 @ 0632</u>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER <u>49</u> °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER
<input checked="" type="checkbox"/> INDICATOR LIGHTS	
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER <u>Repco Marketing Inc</u> LOT # <u>13002</u> EXP. DATE <u>6-19-15</u>	
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) <u>34.0</u> °C SIMULATOR SN <u>SD 2300</u> EXP. DATE <u>1-7-15</u>	

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 = <u>.103</u>	TEST 2 = <u>.104</u>	TEST 3 = <u>.104</u>
----------------------	----------------------	----------------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS <u>0</u> (0-.04)	<u>0</u> (.05-.09)	<u>0</u> (.10-.14)	<u>0</u> (.15-.19)	OVER .19 <u>1</u>
---------------------------	--------------------	--------------------	--------------------	-------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

Operating within DOH & Senior Service Standards

<b>INSPECTING OFFICER</b>	
SIGNATURE <u>Robert G. Kiekerd</u>	PRINT FULL NAME <u>Robert Kiekerd</u>
TYPE II PERMIT NUMBER/EXPIRATION DATE <u>220209, 8-21-14</u>	TELEPHONE NUMBER <u>573-437-2195</u>

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
 2875 James Blvd.  
 Poplar Bluff, MO 63901

**CERTIFICATE OF ANALYSIS**

**MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.**  
**LOT NUMBER: 13002**  
**EXPIRATION DATE: June 19, 2015 at 11:59 p.m.**

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1217 gms/dl +/-0.003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/-3% gms/210L Breath when heated to 34 Degrees Celsius +/-0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is June 20, 2013  
The expiration date for this lot number is June 19, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President  
RepCo Marketing, Inc.

Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
OWENSVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201292  
02/01/14  
06:32


--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM (04-07-2009): OKAY  
HEATERS  
SAMPLE CHAMBER: 49c  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJK  
LMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstu  
vwxyz{|}~`

Operator Signature



Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
OWENSVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201292  
02/01/14

TESTING OFFICER:  
RICKERD/ROBERT  
OFFICER I.D.: 101  
PERMIT NUMBER: 220209  
EXPIRATION DATE: 08/21/14  
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---

BLANK TEST	.000	06:34
INTERNAL STANDARD	VERIFIED	06:34
EXTERNAL STANDARD	.103	06:34
BLANK TEST	.000	06:35
EXTERNAL STANDARD	.104	06:35
BLANK TEST	.000	06:36
EXTERNAL STANDARD	.104	06:36
BLANK TEST	.000	06:37

N = 3  
SIM. = .1  
AVG. = .1036

Operator Signature

*Richard*

2208-02

Face This Side Down - This Edge In First

**BAC DataMaster**  
**Evidence Ticket**

STATE OF MISSOURI  
OWENSVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201292  
02/01/14

ARREST TIME: 06:11

SUBJECT NAME:

WELK/TIM

DOB: 09/09/11      SEX: M

STATE/D.L.: MO/111333222

ARRESTING OFFICER:

RICKERD/ROBERT

OFFICER I.D.: 101

TESTING OFFICER:

RICKERD/ROBERT

OFFICER I.D.: 101

PERMIT NUMBER: 200209


EXPIRATION DATE: 08/21/14

MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST	.000	06:39
INTERNAL STANDARD	VERIFIED	06:39
RADIO INTERFERENCE		

Operator Signature

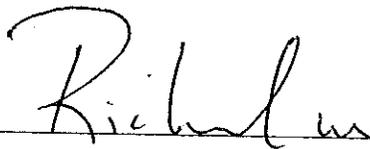

2208-02

State of Missouri  
DEPARTMENT OF HEALTH



P E R M I T  
TYPE II



ROBERT RICKERD

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

**DATAMASTER**


for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

Date 08/21/2012

Number 220209

Expires 08/21/2014

MO 580-0771 (7-85)

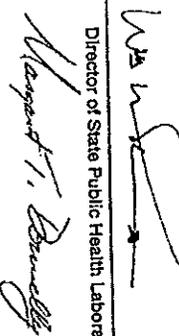  
Director of State Public Health Laboratory

Director, Department of Health

Lab. 4 (R7-86)