



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

**RECEIVED**  
 By Carol Day at 8:51 am, Nov 04, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201299	NAME OF AGENCY Glendale Police Department	DATE OF INSPECTION 11/03/2014
LOCATION OF INSTRUMENT (STREET AND CITY) Glendale Police Department, 424 N. Sappington Road, Glendale, MO 63122		TIME OF INSPECTION 12:45 pm

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 11/03/14 12:45
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER GUTH Laboratories, Inc. LOT # 14200 EXP. DATE 08/05/2016

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN SD2291 EXP. DATE 07/14/2015

CALIBRATION CHECK – (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 ← .098	TEST 2 ← .099	TEST 3 ← .099
---------------	---------------	---------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	0	(0-.04)	0	(.05-.09)	0	(.10-.14)	0	(.15-.19)	0	OVER .19	0
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

Instrument operates within Department of Health specifications.

**INSPECTING OFFICER**

SIGNATURE <i>Robert A. Catlett</i>	PRINT FULL NAME Captain Robert A. Catlett, Jr.
TYPE II PERMIT NUMBER/EXPIRATION DATE 230014 02/08/2015	TELEPHONE NUMBER (314) 965-0000

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
 2875 James Blvd.  
 Poplar Bluff, MO 63901

**BAC DataMaster**  
Evidence Ticket

STATE OF MISSOURI  
GLENDALE POLICE DEPARTMENT

BAC DATA MASTER SERIAL NUMBER 201299  
11/03/14  
12:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM (04-07-2009): OKAY  
HERTERS: 49C  
SAMPLE CHAMBER: OKAY  
FLOW DETECTOR: OKAY  
PUMP: OKAY  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcdefg hijklmno  
pqrstuvwxyz{|}~

Operator Signature 

2208-02

**BAC DataMaster**  
Evidence Ticket

STATE OF MISSOURI  
GLENDALE POLICE DEPARTMENT

BAC DATA MASTER SERIAL NUMBER 201299  
11/03/14


TESTING OFFICER:

CATLETT/ROBERT/H  
OFFICER I.D.: 193  
PERMIT NUMBER: 230014  
EXPIRATION DATE: 02/08/15  
MISCELLANEOUS DATA:  
MONTHLY MAINTENANCE REPORT  
NOVEMBER 2014

--- SUPERVISOR MODE ---

BLANK TEST .000 12:48  
INTERNAL STANDARD .098 12:48  
EXTERNAL STANDARD .000 12:48  
BLANK TEST .000 12:49  
EXTERNAL STANDARD .099 12:49  
BLANK TEST .000 12:50  
EXTERNAL STANDARD .099 12:50  
BLANK TEST .000 12:51

H = 3  
SIM = .1  
RMG = .0986

Operator Signature 

2208-02

**BAC DataMaster**  
Evidence Ticket

STATE OF MISSOURI  
GLENDALE POLICE DEPARTMENT

BAC DATA MASTER SERIAL NUMBER 201299  
11/03/14

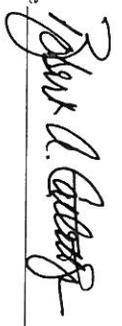
ARREST TIME: 12:00

SUBJECT NAME:  
TEST  
DOB: 01/01/01 SEX: M  
STATE/D.L.: MO/TEST  
ARRESTING OFFICER:  
TEST

OFFICER I.D.: TEST  
TESTING OFFICER:  
CATLETT/ROBERT/H  
OFFICER I.D.: 193  
PERMIT NUMBER: 230014  
EXPIRATION DATE: 02/08/15  
MISCELLANEOUS DATA:  
MONTHLY MAINTENANCE REPORT  
RFI TEST - NOVEMBER 2014

--- BREATH ANALYSIS ---

RADIO INTERFERENCE

Operator Signature 

2208-02



**GUTH LABORATORIES, INC.**

590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

## CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 14200 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on August 6, 2014, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1213% (w/vol) ethyl alcohol. The expiration date for this lot number is August 5, 2016 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.


The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
GUTH LABORATORIES, INC.

*NIST Traceability:*

*Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.*

*All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.*



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

2

PERMIT  
 TYPE II

ROBERT A CATLETT JR

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 02/08/2013

NUMBER 230014

EXPIRES 02/08/2015

MO 380 (3/71 (6-10)

*W. S. R.*  
 DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Sharon Vandenberg*  
 Acting Director,  
 DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES