



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

RECEIVED
By Carol Day at 2:12 pm, Jun 26, 2014

DATAMASTER MAINTENANCE REPORT

REPORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 204086	NAME OF AGENCY MSHP	DATE OF INSPECTION 06/15/2014
LOCATION OF INSTRUMENT (STREET AND CITY) U.S. 160, WEST OF FR 156		TIME OF INSPECTION 2:30 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 6/15/2014 02:33
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER REPCO MARKETING LOT # 12002 EXP. DATE 08/29/2014

SIMULATOR TEMP (34°C ± 0.2°C) 34.1 °C SIMULATOR SN G11068 EXP. DATE 02/14/2015

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

- 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
- 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
- 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 .102	TEST 2 .102	TEST 3 .102
--------------	--------------	--------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	0	(0-.04)	0	(.05-.09)	0	(.10-.14)	2	(.15-.19)	0	OVER .19	1
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

N/A

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME RUSSELL J. FILLIPI
TYPE II PERMIT NUMBER/EXPIRATION DATE 240049 08/07/2016	TELEPHONE NUMBER (417) 895-6868

RETURN COMPLETED REPORT TO THE:
Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
2875 James Blvd.
Poplar Bluff, MO 63901

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.

LOT NUMBER: 12002

EXPIRATION DATE: August 29, 2014 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 12002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1209 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is August 30, 2012
The expiration date for this lot number is August 29, 2014 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

2

**PERMIT
TYPE II**

RUSSELL J FILLIPI

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 3/7/2014

NUMBER 240049

EXPIRES 3/7/2016

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (8-10)

LAB 4 (R6-10)



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator FILLIPI, RUSSELL
Permit No 240049
Date Issued 3/7/2014 Date Expires 3/7/2016

Face This Side Down - This Edge In First


**BAC DataMaster
Evidence Ticket**

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204006
06/15/14

ARREST TIME: 02:00
SUBJECT NAME:
DEAN/LK
DOB: 01/01/68 SEX: M
STATE/D.L.: MO/123456
ARRESTING OFFICER:
FILLIPI/RJ
OFFICER I.D.: 0352
TESTING OFFICER:
SAME
OFFICER I.D.: 352
PERMIT NUMBER: 240049
EXPIRATION DATE: 03/07/16
MISCELLANEOUS DATA:
RFI

--- BREATH ANALYSIS ---

BLANK TEST .000 02:46
INTERNAL STANDARD VERIFIED 02:47
RADIO INTERFERENCE

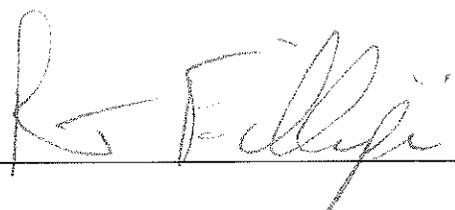

or Signature

Face This Side Down - This Edge In First

**BAC DataMaster
Evidence Ticket**


MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204006
06/15/14
02:33

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM (04-07-2009): OKAY
HEATERS
SAMPLE CHAMBER: 49c
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefg|hijklmno
pqrstuvwxyz{|}~"

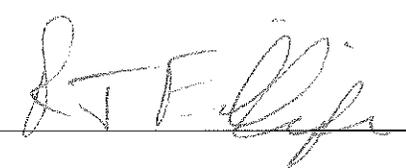

Operator Signature

Face This Side Down - This Edge In First

BAC DataMaster Evidence Ticket

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204086
06/15/14

TESTING OFFICER:
FILLIPI/RJ
OFFICER I.D.: 0352
PERMIT NUMBER: 240049
EXPIRATION DATE: 03/07/16
MISCELLANEOUS DATA:
.10

--- SUPERVISOR MODE ---

BLANK TEST	.000	02:30
INTERNAL STANDARD	VERIFIED	02:38
EXTERNAL STANDARD	.102	02:38
BLANK TEST	.000	02:39
EXTERNAL STANDARD	.102	02:46
BLANK TEST	.000	02:40
EXTERNAL STANDARD	.102	02:43
BLANK TEST	.000	02:41

N = 3
S.D. = .1
AVG. = .102

Operator Signature

