



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED
 By Carol Day at 2:14 pm, Feb 21, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

| | | |
|---|---|---------------------------------|
| DATAMASTER SN 204116 | NAME OF AGENCY Missouri State Highway Patrol | DATE OF INSPECTION 2/19/2014 |
| LOCATION OF INSTRUMENT (STREET AND CITY) Howell County Sheriff's Office, West Plains, Missouri 65775 | | TIME OF INSPECTION 20:40 |

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

| | |
|--|---|
| <input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED) | DATE AND TIME (from printout) 2/19/14 20:40hrs |
| <input checked="" type="checkbox"/> COMPUTER | <input checked="" type="checkbox"/> DETECTOR |
| <input checked="" type="checkbox"/> PROGRAM | <input checked="" type="checkbox"/> FILTERS |
| <input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49 °C | <input checked="" type="checkbox"/> QUARTZ STANDARD |
| <input checked="" type="checkbox"/> FLOW DETECTOR | <input checked="" type="checkbox"/> CALIBRATION |
| <input checked="" type="checkbox"/> PUMP HIGH SPEED | <input checked="" type="checkbox"/> PRINTER |

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Repro Marketing Inc LOT # 13001 EXP. DATE 3-7-15

SIMULATOR TEMP (34°C ± 0.2°C) 34.02 °C SIMULATOR SN G11109 EXP. DATE 4-3-2014

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

- 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
- 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
- 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 = .098 TEST 2 = .098 TEST 3 = .098

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

| | | | | | | | | | | | |
|----------|---|---------|---|-----------|---|-----------|---|-----------|---|----------|---|
| REFUSALS | 1 | (0-.04) | 0 | (.05-.09) | 0 | (.10-.14) | 1 | (.15-.19) | 1 | OVER .19 | 1 |
|----------|---|---------|---|-----------|---|-----------|---|-----------|---|----------|---|

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

Repro Marketing Inc., Lot# 13001, Bottle# 498, Manufactured Date 3/8/13, Exp. Date 3/7/15,
 Ethanol Concentration 0.100%
 This Instrument is Operating In Accordance With DHSS Specifications.

INSPECTING OFFICER

| | |
|---|--|
| SIGNATURE | PRINT FULL NAME Thomas E. Young III |
| TYPE II PERMIT NUMBER/EXPIRATION DATE 220321 Exp. Date 9/29/14 | TELEPHONE NUMBER (417) 469-3121 |

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
 2875 James Blvd.
 Poplar Bluff, MO 63901

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.
LOT NUMBER: 13001
EXPIRATION DATE: March 7, 2015 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 13001 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1215 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is March 8, 2013
The expiration date for this lot number is March 7, 2015 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President

RepCo Marketing, Inc.

State of Missouri
DEPARTMENT OF HEALTH



P E R M I T
TYPE II



THOMAS E YOUNG III

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air. Issued under the provisions of sections 577.020 through 577.041, RSMo 1986.

Date 09/28/2012

Number 220321

Expires 09/28/2014

Director of State Public Health Laboratory

Director, Department of Health

**BAC DataMaster
Evidence Ticket**

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204116
02/19/14
20:40

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM (04-07-2009): OKAY
HEATERS
SAMPLE CHAMBER: 49c
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHI
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopq
rstuvwxyz{|}~

**BAC DataMaster
Evidence Ticket**

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204116
02/19/14


TESTING OFFICER:
YOUNG/T/E
OFFICER I.D.: 749
PERMIT NUMBER: 220321
EXPIRATION DATE: 09/29/14
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---


| | | |
|-------------------|----------|-------|
| BLANK TEST | .000 | 20:43 |
| INTERNAL STANDARD | VERIFIED | 20:43 |
| EXTERNAL STANDARD | .098 | 20:44 |
| BLANK TEST | .000 | 20:44 |
| EXTERNAL STANDARD | .098 | 20:45 |
| BLANK TEST | .000 | 20:45 |
| EXTERNAL STANDARD | .098 | 20:46 |
| BLANK TEST | .000 | 20:46 |

N = 3
SYM. = .1
AVG. = .098

Operator Signature

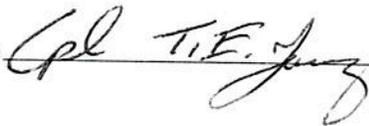

Supervisor Signature

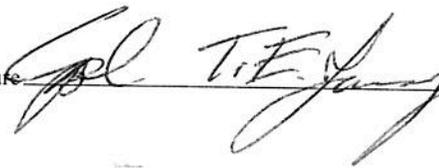

Face This Side ~~Down~~ - This Edge In First

BAC DataMaster
Evidence Ticket

MISSOURI STATE HIGHWAY PATROL
BAC DATAMASTER SERIAL NUMBER 204116
02/19/14

ARREST TIME: 20:15
SUBJECT NAME:
YOUNG/T/E
DOB: 09/12/80 SEX: M
STATE/D.L.: MO/123456
ARRESTING OFFICER:
YOUNG/T/E
OFFICER I.D.: 749
TESTING OFFICER:
YOUNG/T/E
OFFICER I.D.: 749
PERMIT NUMBER: 220321
EXPIRATION DATE: 09/29/14
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

| | | |
|--------------------|----------|-------|
| BLANK TEST | .000 | 20:49 |
| INTERNAL STANDARD | VERIFIED | 20:49 |
| RADIO INTERFERENCE | | |

Operator Signature

