MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

RECEIVED
By Carol Day at 8:44 am, Oct 29, 2014

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN	NAME OF AGENCY	DATE OF INSPECTION
500217	KIMBERLING CITY PD	10/28/2014
LOCATION OF INSTRUMENT (STREET AND CITY)		TIME OF INSPECTION
34 KIMBERLING BLVD KIMBERLING CITY, MO 65686		15:12:05

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

☒ DIAGNOSTIC RECORD

DATE AND TIME 10/28/2014 15:12:07

☒ DETECTOR
☒ PROGRAM
☒ FILTER 1
☒ SAMPLE CHAMBER 48.9°C
☒ FILTER 2
☒ BREATH TUBE 48.1°C
☒ FILTER 3
☒ PUMP
☒ INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

☒ SIMULATOR STANDARD
☐ COMPRESSED ETHANOL-GAS MIXTURE

☒ STANDARD SUPPLIER GUTH LOT # 14200 EXP. DATE 08/05/2016

☒ SIMULATOR TEMP (34°C ± 0.2°C) 34.0 SIMULATOR SN SD2753 SIMULATOR EXP DATE 10/06/2015

☒ CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

☒ 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
☐ 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
☐ 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.099	TEST 2: 0.099	TEST 3: 0.099

☒ PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE	PRINT FULL NAME	
	AARON P HOEFT	
TYPE II PERMIT NUMBER	EXPIRATION DATE	TELEPHONE NUMBER
240370	10/17/2016	417-739-2131

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901

AN EQUAL OPPORTUNITY/AFFIRMATIVE ACTION EMPLOYER
services provided on a nondiscriminatory basis

MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES

BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11

LOCATION OF INSTRUMENT	INSTRUMENT SERIAL NUMBER	DATE OF TEST	TIME OF TEST
34 KIMBERLING BLVD KIMBERLING CITY, MO 65686	500217	10/28/2014	15:25:56

SUBJECT NAME	DATE OF BIRTH
TEST B BLANK	07/21/1981

SEX	SUBJECT DRIVER'S LICENSE NUMBER	STATE
M	1025252	MO

ARRESTING OFFICER	ARRESTING OFFICER ID
AARON P HOEFT	903

OPERATOR	OPERATOR PERMIT	PERMIT EXP DATE
AARON HOEFT	240370	10/17/2016

OPERATIONAL CHECKLIST: INTOX DMT

- ☒ 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- ☒ 2. Subject observed for at least 15 minutes by AARON HOEFT. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- ☒ 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- ☒ 4. Press the Run button on the display screen.
- ☒ 5. Enter subject and officer information.
- ☒ 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	15:26
INTERNAL STANDARD	VERIFIED	15:27
SUBJECT SAMPLE (Vol=3.38L)	0.000	15:27
BLANK TEST	0.000	15:28

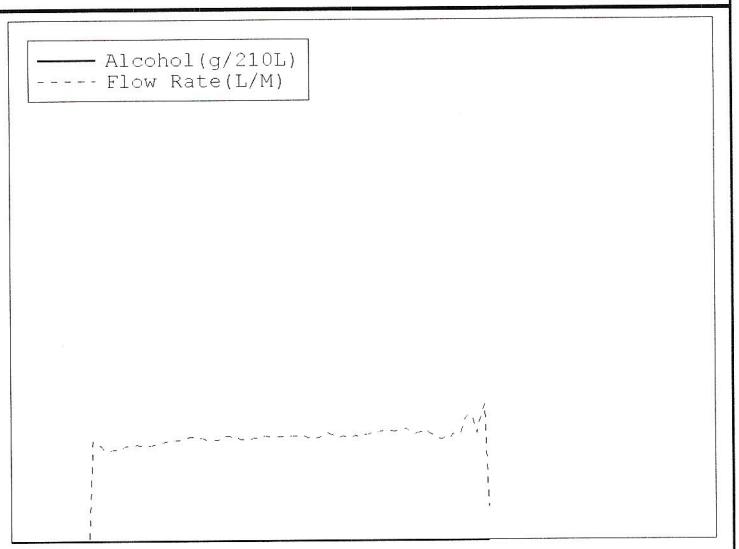

COMMENTS

blank monthly test

CERTIFICATION BY OPERATOR

BAC: 0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- ☒ 1. There was no deviation from the procedure approved by the department.
- ☒ 2. To the best of my knowledge the instrument was functioning properly.
- ☒ 3. I am authorized to operate the instrument.
- ☒ 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR	DATE
	10/28/2014
WITNESS (IF ANY)	DATE
	10/28/2014

AN EQUAL OPPORTUNITY/AFFIRMATIVE ACTION EMPLOYER
services provided on a nondiscriminatory basis

STATE OF MISSOURI

DEPARTMENT OF HEALTH AND SENIOR SERVICES

BREATH ALCOHOL PROGRAM

2

PERMIT

TYPE II

AARON P HOEFT

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 10/17/2014

NUMBER 240370

EXPIRES 10/17/2016

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

Gail Vasterling ,acting director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

Simulator Calibration Report

This calibration report is to certify the alcohol reference simulator listed below has been examined and tested using standards traceable to the National Institute of Standards and Technology (NIST) in accordance with the standards set by the Missouri Department of Health and Senior Services Rules and Regulations: 19 CSR 25-30.051 (4).

Checked:10/06/2014 Expires:**10/06/2015**
MSC Tech: DRL
Temp: 33.99 Digital Therm. SN: 093752
Agency: Kimberling City Police Dept.
SD 2753

Technician Printed Name: DAN LUCAS

Technician Signature: [signature]

Date: 10/6/14

Contact: Missouri Safety Center

Breath-Alcohol Instrument Training Program

660-543-4834

GUTH LABORATORIES, INC.
590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number **14200** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on **August 6, 2014,** using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.1213%** (w/vol) ethyl alcohol. The expiration date for this lot number is **August 5, 2016** at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of **0.100 g/210L +/- 3%.**

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President
GUTH LABORATORIES, INC.

NIST Traceability:
*Testing was conducted using Cerilliant Reference Standard lot number **FN122211-02** whose values are traceable to NIST.*
All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.