



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
 INTOX DMT MAINTENANCE REPORT

RECEIVED

REPORT #1

By Carol Day at 2:16 pm, Jan 06, 2015

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500225	NAME OF AGENCY Trenton Police Department	DATE OF INSPECTION 12/29/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 610 Main Street, Trenton, Missouri 64683		TIME OF INSPECTION 22:42:54

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>12/29/2014 22:42:56</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>42.8°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS		
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE	
<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETER</u>	LOT # <u>AG418902</u>	EXP. DATE <u>07/08/2016</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C)	SIMULATOR SN	SIMULATOR EXP DATE

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.099	TEST 2: 0.099	TEST 3: 0.098
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:					
REFUSALS: 1	0-.04: 1	.05-.09: 1	.10-.14: 2	.15-.19: 3	OVER .19: 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Matt Preston #106

INSPECTING OFFICER	
SIGNATURE 	PRINT FULL NAME MATTHEW W PRESTON
TYPE II PERMIT NUMBER 240413	EXPIRATION DATE 11/20/2016
TELEPHONE NUMBER 660-359-5557	

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901

STANDARD CHANGE

Trenton Police Department
INTOX dmt: 500225

Date: 12/29/2014
Time: 22:52:58


OPERATOR NAME:
MATTHEW W PRESTON
PERMIT NUMBER: 240413
EXPIRATION DATE: 11/20/2016

LOT #: AG418902
SUPPLIER: INTOXIMETER
EXPIRATION: 07/08/2016
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.099

BLANK TEST	0.000	22:53
INTERNAL STANDARD	VERIFIED	22:54
EXTERNAL STANDARD	0.099	22:54
BLANK TEST	0.000	22:55

Average = 0.0990
Std Dev = 0.0000
Spread = 0.0000

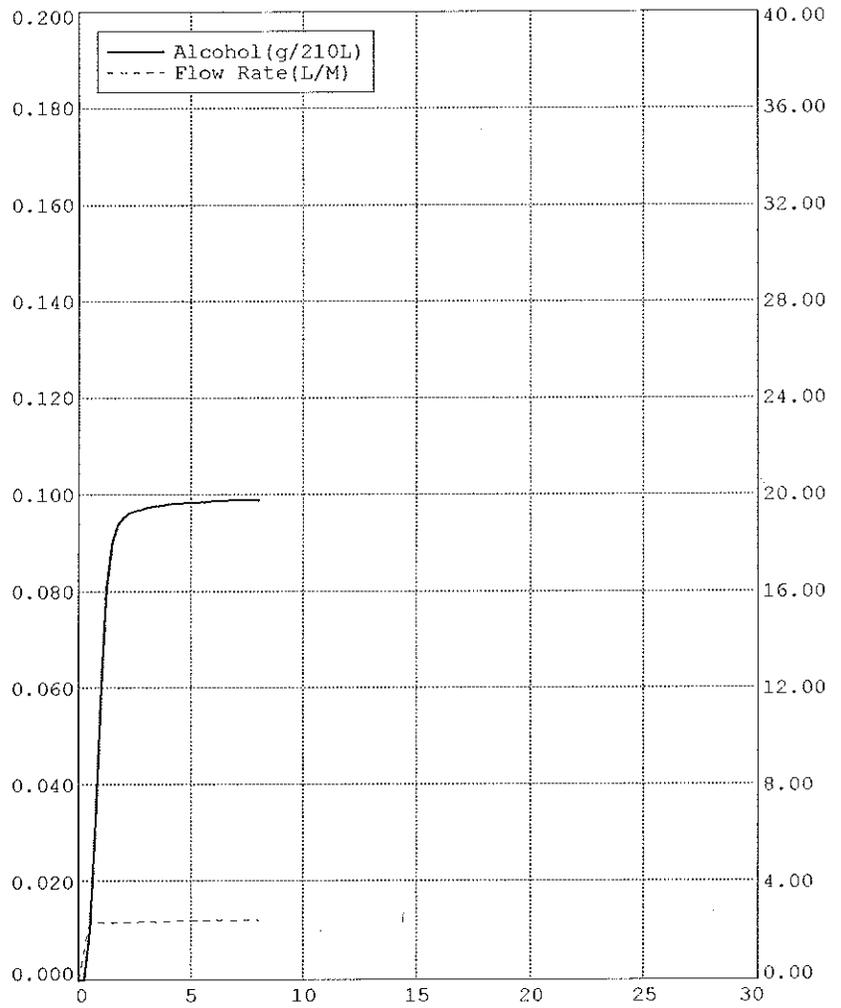



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

**PERMIT
 TYPE II**

MATTHEW W PRESTON

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 11/20/2014

NUMBER 240413

EXPIRES 11/20/2016

MO 580-0771 (6-10)

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

,acting director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator PRESTON, MATTHEW
 Permit No 240413
 Date Issued 11/20/2014 Date Expires 11/20/2016