



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
CMI INTOXILYZER 8000 MAINTENANCE REPORT

RECEIVED
 By Carol Day at 8:42 am, Mar 17, 2014 #2

Complete this report in duplicate at the time of the regular monthly preventive maintenance check, and whenever instrument is repaired. Send one copy to Department of Health and Senior Services, and retain one copy in department file.

| | | | |
|---------------------------------------|---|----------------------------------|-----------------------------|
| INSTRUMENT SERIAL NUMBER 80-005838 | LOCATION OF INSTRUMENT KCMO POLICE DEPT. | DATE OF INSPECTION 03/08/2014 | TIME OF INSPECTION 15:13 |
|---------------------------------------|---|----------------------------------|-----------------------------|

| CALIBRATION CHECK RESULTS | | | CALIBRATION CHECK SUMMARY | | |
|---------------------------|--------|-------|---|--|--|
| Test | g/210L | Time | STANDARD TYPE DRY | STANDARD LOT # 21713080 | STANDARD EXPIRATION DATE 09/01/2015 |
| Air Blank | 0.000 | 15:14 | SIM TEMPERATURE N/A | SIM SERIAL NUMBER N/A | SIM CERTIFICATE EXPIRATION N/A |
| Cal Check | 0.080 | 15:15 | STANDARD VALUE 0.080 | STANDARD SUPPLIER CMI | |
| Air Blank | 0.000 | 15:15 | CALIBRATION CHECK RESULT 1 0.080 | | |
| Cal Check | 0.080 | 15:15 | CALIBRATION CHECK RESULT 2 0.080 | | |
| Air Blank | 0.000 | 15:16 | CALIBRATION CHECK RESULT 3 0.080 | | |
| Cal Check | 0.080 | 15:16 | MAXIMUM DEVIATION (MUST BE WITHIN 5%) 0.0% | SPREAD (MUST BE .005 OR LESS) 0.000 | |
| Air Blank | 0.000 | 15:17 | <h1>Pass</h1> | | |


| DIAGNOSTIC TEST RESULTS | | | RFI TEST RESULTS | | |
|-----------------------------|------|--|------------------|--------|-------|
| Voltage/Current Test | Pass | | Test | g/210L | Time |
| RAM Test | Pass | | Air Blank | 0.000 | 15:17 |
| EEPROM Checksum Test | Pass | | Subject Test | RFI* | 15:18 |
| Real Time Clock Test | Pass | | Air Blank | 0.000 | 15:18 |
| DSP Test | Pass | | <h1>Pass</h1> | | |
| Analytical Stability Test | Pass | | | | |
| Modem Test | Pass | | | | |
| Temperature Regulation Test | Pass | | <h1>Pass</h1> | | |

| NUMBER OF REFUSALS AND SUBJECT BREATH TESTS IN EACH RANGE SINCE LAST MAINTENANCE REPORT | | | | | | | |
|---|---------|---------|---------|---------|----------|--|--|
| REFUSALS | .00-.04 | .05-.09 | .10-.14 | .15-.19 | OVER .19 | | |
| 3 | 0 | 0 | 3 | 0 | 2 | | |

List any new parts and describe any alteration or modification that was made to restore the instrument to operate satisfactorily and within established limits (use other side if necessary).

TESTED AND CERTIFIED WITHIN DEPARTMENT OF HEALTH AND SENIOR SERVICES
 TESTED AND CERTIFIED WITHIN DEPARTMENT OF HEALTH AND SENIOR SERVICES G
 UIDELINES

| | | |
|--|-------------------------------|--------------------------------|
| INSPECTING OFFICER | | |
| SIGNATURE <i>P. O. Smeska #5200</i> | PRINT NAME KORI SMEISKA | |
| TYPE II PERMIT NUMBER 230169 | EXPIRATION DATE 08/14/2015 | TELEPHONE NUMBER 8162345000 |

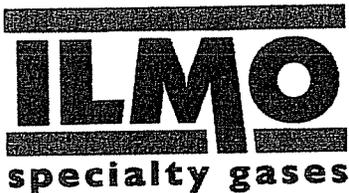

7 Eastgate Dr. • P.O. Box 790 • Jacksonville, IL 62651-0790
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

Certificate of Analysis


Certificate ID: 5288
Part #: BAC105L080T
Cylinder Size: 105L
Lot Number: 21713080A1
Expiration: 9/1/2015

0.080 BAC (For use with breath alcohol testing instruments)

Contents: 105 Liters @ 1000 psig 70°F (21°C)

| Component: | Concentration: | Accuracy: | Method: |
|------------|----------------|--------------------------|---------|
| Ethanol | 208.4 ppm | +/- 0.002 or 2% | NDIR |
| Nitrogen | Balance | BAC whichever is greater | |

*NIST Standard Reference Material
Cylinder No. CC14290 / Job No. 09160202
Certified 212.8 µmol/mol Ethanol in Nitrogen
for ILMO Products Co., Jacksonville, IL

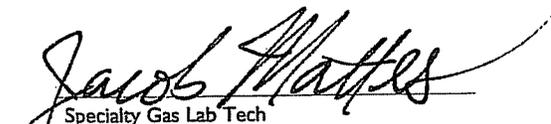
Specialty Gas Lab Tech

08/16/13
Date

Distributed by: CMI Inc.
316 East Ninth Street
Owensboro, KY 42303
Phone 866-835-0690
www.alcoholtest.com

