

MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
 DATAMASTER MAINTENANCE REPORT

RECEIVED

By Carol Day at 11:59 am, Nov 20, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 940230	NAME OF AGENCY Canton Police Department	DATE OF INSPECTION 11/07/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 108 North 6th Street, Canton		TIME OF INSPECTION 00:24 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 11/07/14 00:24
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER _____ 48°C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Guth Laboratories Inc LOT # 13280 EXP. DATE 10/16/2015

SIMULATOR TEMP (34°C ± 0.2°C) 34 °C SIMULATOR SN 93752 EXP. DATE 05/15/2015

CALIBRATION CHECK -- (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.040% STANDARD - MUST READ BETWEEN 0.036% AND 0.042% INCLUSIVE

TEST 1 μ .102	TEST 2 μ .100	TEST 3 μ .099
-------------------	-------------------	-------------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	0	(0-.04)	0	(.05-.09)	0	(.10-.14)	0	(.15-.19)	1	OVER .19	0
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).
 Datamaster 940230 complies with the Department of Health and Senior Services rules and regulations

INSPECTING OFFICER	
SIGNATURE 	PRINT FULL NAME Don L Cibert
TYPE II PERMIT NUMBER/EXPIRATION DATE 240364 10/17/2016	TELEPHONE NUMBER (573) 655-4099

RETURN COMPLETED REPORT TO THIS: **Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office**
 2875 James Blvd.
 Poplar Bluff, MO 63901



GUTH LABORATORIES, INC.

599 NORTH 87th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-584-5170

CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 13280 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on October 18, 2013, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1217% (w/vol) ethyl alcohol. The expiration date for this lot number is October 16, 2015 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President
GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
CANTON POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 940220
11/07/14
00124


--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM (04-07-2009): OKAY
SEETERS
SAMPLE CHAMBER: 18c
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20
ABCDEFGHIJKLMN OPQRSTUVWXYZ [] ^ _ ` abcdefghijklmnop
pqrs tuvwxyz 0123456789

Operator Signature

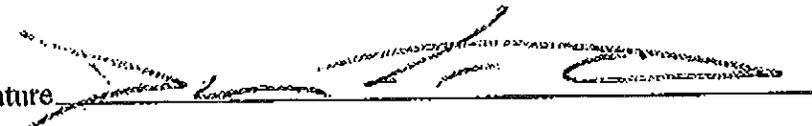

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
CANTON POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 946206
11/07/14


TESTING OFFICER:
CIVERT/DONAL
OFFICER I.D.# 112
SERIAL NUMBER: 240364
EXPIRATION DATE: 10/17/16
EXCESSIVE DATA:
MONTHLY MAINTENANCE

SUPERVISOR MODE

BLANK TEST	.000	00:27
INTERNAL STANDARD	VERIFIED	00:27
INTERNAL STANDARD	.100	00:29
BLANK TEST	.000	00:29
INTERNAL STANDARD	.100	00:29
BLANK TEST	.000	00:30
INTERNAL STANDARD	.099	00:31
BLANK TEST	.000	00:31

N = 8
S.D. = .1
AVG. = .1003

Operator Signature

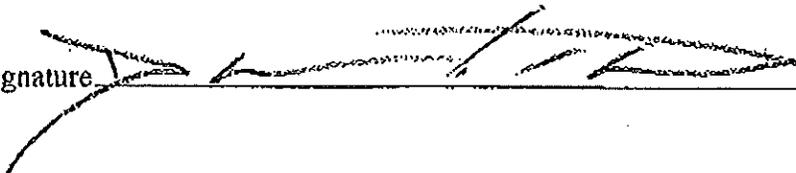

**BAC DataMaster
Evidence Ticket**

STATE OF MISSOURI
CANTON POLICE DEPARTMENT

SAC DATAMASTER SERIAL NUMBER 840230
11/07/14

ARREST TIME: 00:00
SUBJECT NAME:
RFI TEST
DOB: 11/11/11 SEX: M
STATE D.L. NO: 1111111111
ARRESTING OFFICER:
N/A
OFFICER I.D. #: N/A
TESTING OFFICER:
GIBERT/DONALD
OFFICER I.D. #: 112
PERMIT NUMBER: 840264
EXPIRATION DATE: 10/17/16
MISCELLANEOUS DATA:
RFI TEST
MONTHLY MAINTENANCE

--- BREATH ANALYSIS ---

BLANK TEST	.000	00:45
INTERNAL STANDARD	VERIFIED	00:43
RADIO INTERFERENCE		

Operator Signature _____



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II

DON L CIBERT

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 10/17/2014

NUMBER 240364

EXPIRES 10/17/2016

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

acting director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES