



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

**RECEIVED**  
 By Carol Day at 10:55 am, Jan 22, 2014

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 940234	NAME OF AGENCY Crocker Police Department	DATE OF INSPECTION 01/18/2014
LOCATION OF INSTRUMENT (STREET AND CITY) 108 S Commercial Street, Crocker MO 65452		TIME OF INSPECTION 5:28 pm

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 01/18/2014 5:28pm
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 47 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Rep Co Marketing Inc LOT # 12002 EXP. DATE 08/29/2014

SIMULATOR TEMP (34°C ± 0.2°C) 34 °C SIMULATOR SN SD2729 EXP. DATE 08/28/2014

CALIBRATION CHECK – (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1  .098	TEST 2  .099	TEST 3  .099
--------------	--------------	--------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

**INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)**

REFUSALS	0	(0-.04)	1	(.05-.09)	1	(.10-.14)	0	(.15-.19)	0	OVER .19	0
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

<b>INSPECTING OFFICER</b>	
SIGNATURE 	PRINT FULL NAME Aaron Baker
TYPE II PERMIT NUMBER/EXPIRATION DATE 230112 06/12/2015	TELEPHONE NUMBER (573) 736-2211

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
 2875 James Blvd.  
 Poplar Bluff, MO 63901

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.

LOT NUMBER: 12002

EXPIRATION DATE: August 29, 2014 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 12002 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1209 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.


This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is August 30, 2012  
The expiration date for this lot number is August 29, 2014 at  
11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President  
RepCo Marketing, Inc.



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

2

**PERMIT  
TYPE II**

**AARON J BAKER**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 06/12/2013

NUMBER 230112

EXPIRES 06/12/2015

*W. W. ...*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Paul Vesterly*  
Acting Director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
CROCKER POLICE DEPARTMENT


BAC DATAMASTER SERIAL NUMBER 940034  
01/13/14

TESTING OFFICER:  
BAKER/ARRON/J  
OFFICER I.D.: 596  
PERMIT NUMBER: 808112  
EXPIRATION DATE: 06/12/15  
MISCELLANEOUS DATA:

--- SUPERVISOR NODE ---

BLANK TEST	.000	17:50
INTERNAL STANDARD	VERIFIED	17:50
EXTERNAL STANDARD	.000	17:52
BLANK TEST	.000	17:51
EXTERNAL STANDARD	.000	17:51
BLANK TEST	.000	17:52
EXTERNAL STANDARD	.000	17:50
BLANK TEST	.000	17:50

N = 3  
SIM. = .1  
AVC. = .0036

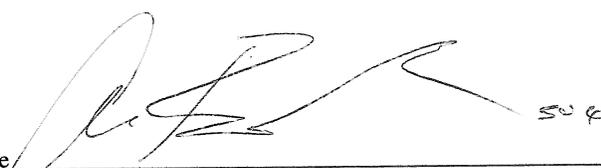

Operator Signature

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
CROCKER POLICE DEPARTMENT


BAC DATAMASTER SERIAL NUMBER 940034  
01/13/14

ARREST TIME: 17:15  
SUBJECT NAME:  
CFITEST  
DOB: 11/11/11 SEX: M  
STATE/D.L.I.: NM/1  
ARRESTING OFFICER:  
NA

OFFICER I.D.: NA  
TESTING OFFICER:  
BAKER/ARRON/J  
OFFICER I.D.: 596  
PERMIT NUMBER: 808112  
EXPIRATION DATE: 06/12/15  
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST	.000	17:39
INTERNAL STANDARD	VERIFIED	17:40
RADIO INTERFERENCE		

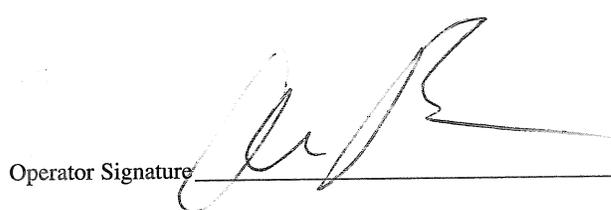

Operator Signature

**BAC DataMaster**  
**Evidence Ticket**

STATE OF MISSOURI  
CROCKER POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 940204  
01/19/14  
17:28

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM (04-07-2009): OKAY

HEATERS  
SAMPLE CHAMBER: 47L

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY


FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#\$%^&\*~`-./0123456789:;|<=>?@BCDEFG  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abdefghijklmnop  
qrstuvwxyz{|}~\*

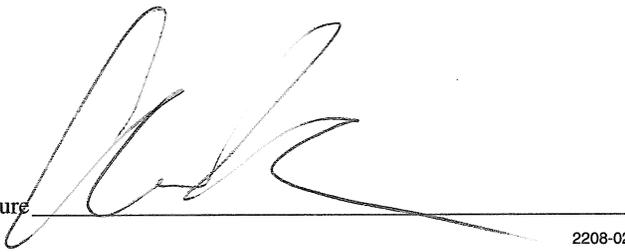

Operator Signature