MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

DATAMASTER MAINTENANCE REPORT

REPORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 3
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into se
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

RECEIVED
By Carol Day at 12:52 pm, Jul 24, 2015

DATAMASTER SN	NAME OF AGENCY	DATE OF INSPECTION
201209	Perryville PD	07/20/2015
LOCATION OF INSTRUMENT (STREET AND CITY)		TIME OF INSPECTION
120 N. Jackson St., Perryville		10:56 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

☑ DIAGNOSTIC CHECK (PRINTOUT ATTACHED) DATE AND TIME (from printout) 07/20/2015 10:56 am

☑ COMPUTER ☑ DETECTOR

☑ PROGRAM ☑ FILTERS

☑ HEATERS SAMPLE CHAMBER +48 °C ☑ QUARTZ STANDARD

☑ FLOW DETECTOR ☑ CALIBRATION

☑ PUMP HIGH SPEED ☑ PRINTER

☑ INDICATOR LIGHTS

☑ SIMULATOR SOLUTION SUPPLIER Repco Marketing LOT # 14001 EXP. DATE 04/30/2016

☑ SIMULATOR TEMP (34°C ± 0.2°C) +34 °C SIMULATOR SN sd2778 EXP. DATE 05/05/2016

☑ CALIBRATION CHECK – (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

☑ 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
☐ 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
☐ 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1	TEST 2	TEST 3
.101	.102	.102

☑ PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT: (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	(0-.04)	(.05-.09)	(.10-.14)	(.15-.19)	OVER .19
0	3	0	0	1	1

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

Instrument is working within DOHSS Guidelines

INSPECTING OFFICER

SIGNATURE	PRINT FULL NAME
Ryan L Worthington	Ryan L. Worthington
TYPE II PERMIT NUMBER/EXPIRATION DATE	TELEPHONE NUMBER
250120 05/14/2017	(573) 547-4546

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
2875 James Blvd.
Poplar Bluff, MO 63901

REPCO MARKETING INC.

9101-108 STONYBROOK DRIVE
RALEIGH, N.C. 27604
919-876-5490

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.
LOT NUMBER: 14001
EXPIRATION DATE: April 30, 2016 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 14001 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1216 gms/dl +/-.003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/-3% gms/210L Breath when heated to 34 Degrees Celsius +/-0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is May 1, 2014. The expiration date for this lot number is April 30, 2016 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.

Cecil B. Garner, President
RepCo Marketing, Inc.

Form RM 02

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201209
07/20/15
10:56

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM (04-07-2009):	OKAY
HEATERS	
SAMPLE CHAMBER:	48c
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

```
 !"#$%&'()*+,-./0123456789:;<=>?@ABCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmno
pqrstuvwxyz{|}~
```

Operator Signature R L Worthington

Printed on recycled paper with agri-based inks

BAC DataMaster
Evidence Ticket

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201209
07/20/15

ARREST TIME: 10:00
SUBJECT NAME:
DOE/JON/B
DOB: 01/01/01 SEX: M
STATE/D.L.: MO/0000000000
ARRESTING OFFICER:
WORTHINGTON/RYAN/L
OFFICER I.D.: 105
TESTING OFFICER:
SAME
OFFICER I.D.: SAME
PERMIT NUMBER: 250120
EXPIRATION DATE: 05/14/17
MISCELLANEOUS DATA:
RFI TEST

---- BREATH ANALYSIS ---

RADIO INTERFERENCE

Operator Signature R J Worthington

Printed on recycled paper with agri-based inks CMSU 2208-02

BAC DataMaster Evidence Ticket

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER.201289
07/20/15

TESTING OFFICER:
WORTHINGTON/RYAN/L
OFFICER I.D.: 105
PERMIT NUMBER: 250120
EXPIRATION DATE: 05/14/17
MISCELLANEOUS DATA:

--- SUPERVISOR MODE ---

BLANK TEST	.000	10:58
INTERNAL STANDARD	VERIFIED	10:58
EXTERNAL STANDARD	.101	10:59
BLANK TEST	.000	10:59
EXTERNAL STANDARD	.102	11:00
BLANK TEST	.000	11:00
EXTERNAL STANDARD	.102	11:01
BLANK TEST	.000	11:01

N = 3
SIM. = .1
AVG. = .1016

Operator Signature R L Worthington

Printed on recycled paper with agri-based inks CMSU 2208-02

STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II

RYAN L WORTHINGTON

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE: 5/14/2015

NUMBER: 250120

EXPIRES: 5/14/2017

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator WORTHINGTON, RYAN
Permit No 250120
Date Issued 6/14/2015 Date Expires 6/14/2017

Simulator Calibration Report

This calibration report is to certify the alcohol reference simulator listed below has been examined and tested using standards traceable to the National Institute of Standards and Technology (NIST) in accordance with the standards set by the Missouri Department of Health and Senior Services Rules and Regulations: 19 CSR 25-30.051 (4).

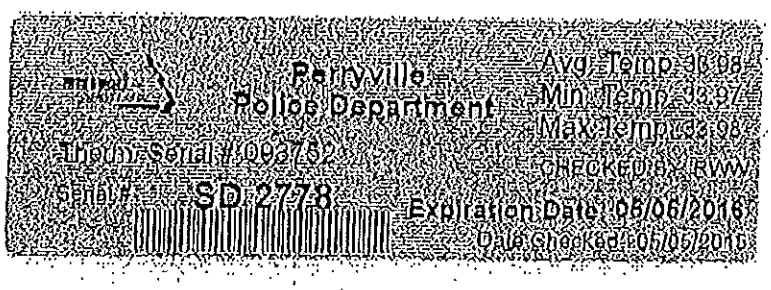

Technician Printed Name: ROBERT WELSH

Technician Signature: [signature]

Date: 05/05/2015

Contact: Missouri Safety Center

Breath-Alcohol Instrument Training Program

660-543-4834