



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

**DATAMASTER MAINTENANCE REPORT**

**RECEIVED**

REPORT #6

By Carol Day at 1:43 pm, Mar 04, 2015

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201259	NAME OF AGENCY Boonville Police Department	DATE OF INSPECTION 03/04/2015
LOCATION OF INSTRUMENT (STREET AND CITY) 401 E. Morgan Street, Boonville MO 65233		TIME OF INSPECTION 0204

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 03/04/15 0253
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 48 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Guth Labs LOT # 14200 EXP. DATE 08/05/16

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN SD3501 EXP. DATE ~~08/05/16~~

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) 09/30/16

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 = .099 TEST 2 = .089 TEST 3 = .100

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS 0	(0-.04) 0	(.05-.09) 1	(.10-.14) 0	(.15-.19) 0	OVER .19 0
------------	-----------	-------------	-------------	-------------	------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME James Deckard
TYPE II PERMIT NUMBER/EXPIRATION DATE 220215 09/04/2014	TELEPHONE NUMBER (660) 882-2727

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
2875 James Blvd.  
Poplar Bluff, MO 63901

**GUTH LABORATORIES, INC.**

699 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-664-6470

**CERTIFICATE OF ANALYSIS**

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 14200 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on August 6, 2014, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1213% (w/vol) ethyl alcohol. The expiration date for this lot number is August 5, 2016 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
GUTH LABORATORIES, INC.

STATE OF MISSOURI - THIS SPACE IS FIRST

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
BOONVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201259  
03/04/15  
02:04

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM (24-67-2009): OKAY

HEATERS  
SAMPLE CHAMBER: 48C

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY


FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJK  
LMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~

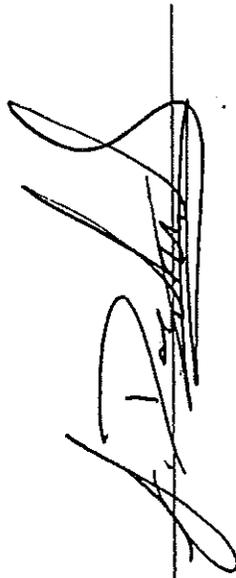

Operator Signature

FACE THIS SIDE DOWN - THIS PAGE IS FIRST

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
BOONVILLE POLICE DEPARTMENT

BAC DATAMASTER SERIAL NUMBER 201259  
03/04/15

TESTING OFFICER:

DECKER/JAMES/W

OFFICER I.D. # 07

PERMIT NUMBER: 240291

EXPIRATION DATE: 06/27/16

MISCELLANEOUS DATA:

--- SUPERVISOR MOU ---

BLANK TEST	.000	02:23
INTERNAL STANDARD	VERIFIED	02:23
EXTERNAL STANDARD	.099	02:24
BLANK TEST	.000	02:24
EXTERNAL STANDARD	.099	02:25
BLANK TEST	.000	02:25
EXTERNAL STANDARD	.100	02:26
BLANK TEST	.000	02:26

N = 3

STD. = .1

PRG. = 0593

Operator Signature

Face This Side Down - This Edge In First

# BAC DataMaster Evidence Ticket

STATE OF MISSOURI  
BOONVILLE POLICE DEPARTMENT

BAC DATA MASTER SERIAL NUMBER 201259  
03/04/15

ARREST TIME: 09:30

SUBJECT NAME:

TEST:

DOB: 01/01/70 SEX: F

STATE/D.L.: MO/00000000

ARRESTING OFFICER:

TEST:

OFFICER I.D.: 000

TESTING OFFICER:

BECKARD, JAMES/M

OFFICER I.D.: 04

PERMIT NUMBER: 240291


EXPIRATION DATE: 06/27/15

MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST .000 02:12  
INTERNAL STANDARD VERIFIED 02:13  
RADIO INTERFERENCE

Operator Signature

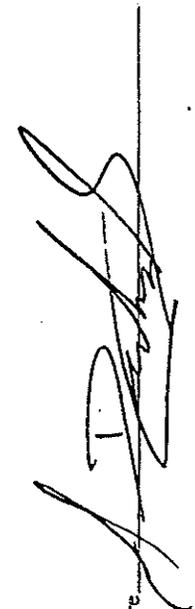



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM



**PERMIT  
TYPE II**

**JAMES M DECKARD**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE: 6/27/2014

NUMBER 240291

EXPIRES 6/27/2016

MO 690-0771 (9-10)

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (9-10)

STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*

Operator **DECKARD, JAMES**  
Permit No **240291**  
Date Issued **6/27/2014** Date Expires **6/27/2016**