



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

RECEIVED

By Carol Day at 7:11 am, Mar 10, 2015

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201270	NAME OF AGENCY La Grange Police Department	DATE OF INSPECTION 05/05/2015 3/5/15 CD
LOCATION OF INSTRUMENT (STREET AND CITY) 204 west Washington Street, La Grange		TIME OF INSPECTION 06:22 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 03/05/15 06:22
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49°C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

<input checked="" type="checkbox"/> INDICATOR LIGHTS
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER Guth Laboratories Inc LOT # 14110 EXP. DATE 05/01/2016
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) 34 °C SIMULATOR SN DR 5388 EXP. DATE 04/29/2015

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 → .100	TEST 2 → .100	TEST 3 → .100
---------------	---------------	---------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS 0	(0-.04) 0	(.05-.09) 0	(.10-.14) 0	(.15-.19) 0	OVER .19 0
------------	-----------	-------------	-------------	-------------	------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS
(USE OTHER SIDE IF NECESSARY).
Datamaster 201270 complies with the Department of Health and Senior Services rules and regulations.

INSPECTING OFFICER	
SIGNATURE ▶	PRINT FULL NAME Don L Cibert
TYPE II PERMIT NUMBER/EXPIRATION DATE 240364 10/17/2016	TELEPHONE NUMBER (573) 655-4099
RETURN COMPLETED REPORT TO THIS:	Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office 2875 James Blvd. Poplar Bluff, MO 63901

**GUTH LABORATORIES, INC.**

590 NORTH 6TH STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

CERTIFICATE OF ANALYSIS**Certified Alcohol Reference Solution for Simulator**

Random Samples of Lot Number 14110 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on May 5, 2014, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1206% (w/vol) ethyl alcohol. The expiration date for this lot number is May 1, 2016 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- .2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President
GUTH LABORATORIES, INC.

NIST Traceability:

Testing was conducted using Cerilliant Reference Standard lot number FN122211-02 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.

FACE THIS SIDE DOWN - THIS EDGE IN FIRST

BAC DataMaster
Evidence Ticket

STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201270
03/05/15
06:22

----- DIAGNOSTIC CHECK -----

COMPUTER: OKAY

PROGRAM (04-07-2009): OKAY

HEATERS
SAMPLE CHAMBER: 49c

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:; <=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnop
qrstuvwxyz{|}~"

OPERATOR SIGNATURE _____

Card Stock No.
60021

REORDER ALL SUPPLIES FROM N.P.A.S.
P.O. BOX 1435, MANSFIELD, OH 44901

T-659 P0003/0007 F-127

5736554528

LAGRANGE POLICE

03-09-'15 11:56 FROM-

EX

FACE THIS SIDE DOWN - THIS EDGE IN FIRST

BAC DataMaster
Evidence Ticket

STATE OF MISSOURI
BAC-DATAMASTER SERIAL NUMBER 201270
03/05/15


TESTING OFFICER:
CIBERT/DON/L
OFFICER I.D.: 112
PERMIT NUMBER: 240364
EXPIRATION DATE: 10/17/16
MISCELLANEOUS DATA:
MONTHLY MAINTENANCE

--- SUPERVISOR MODE ---

BLANK TEST	.000	06:25
INTERNAL STANDARD	VERIFIED	06:25
EXTERNAL STANDARD	.100	06:26
BLANK TEST	.000	06:26
EXTERNAL STANDARD	.100	06:27
BLANK TEST	.000	06:27
EXTERNAL STANDARD	.100	06:28
BLANK TEST	.000	06:28

----- N = 3
----- SIM. = .1
----- AVG. = .1

OPERATOR SIGNATURE



Card Stock No.
60021

REORDER ALL SUPPLIES FROM N.P.A.S.
P.O. BOX 1435, MANSFIELD, OH 44901

FACE THIS SIDE DOWN - THIS EDGE IN FIRST

BAC DataMaster
Evidence Ticket


STATE OF MISSOURI
BAC DATAMASTER SERIAL NUMBER 201270
03/05/15

ARREST TIME: 06:00
SUBJECT NAME:
RFI/TEST
DOB: 11/11/11 SEX: M
STATE/D.L.: MO/111111111
ARRESTING OFFICER:
N/A
OFFICER I.D.: N/A
TESTING OFFICER:
CIBERT/DON/L
OFFICER I.D.: 112
PERMIT NUMBER: 248364
EXPIRATION DATE: 10/17/16
MISCELLANEOUS DATA:
RFI TEST
MONTHLY MAINTENANCE

----- BREATH ANALYSIS -----

.....	BLANK TEST	.000	06:31
_____	INTERNAL STANDARD	VERIFIED	06:31
	RADIO INTERFERENCE		

OPERATOR SIGNATURE

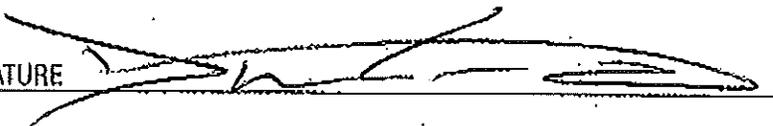



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
DON L CIBERT

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 10/17/2014

NUMBER 240364

EXPIRES 10/17/2016

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

acting director

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)