



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

RECEIVED

By Carol Day at 12:23 pm, Jul 06, 2015

Complete this report at the time of the regular monthly preventive maintenance check
 Complete this report whenever the instrument is serviced or repaired and whenever it
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DH

INTOX DMT SN 500266	NAME OF AGENCY University of Missouri Police Department	DATE OF INSPECTION 07/04/2015
LOCATION OF INSTRUMENT (STREET AND CITY) 901 Virginia Ave, Columbia		TIME OF INSPECTION 04:43:50

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>07/04/2015 04:43:52</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.8°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG429701 EXP. DATE 10/24/2016

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.077 TEST 2: 0.076 TEST 3: 0.076

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: <u>2</u>	0-.04: <u>11</u>	.05-.09: <u>5</u>	.10-.14: <u>4</u>	.15-.19: <u>2</u>	OVER .19: <u>1</u>
--------------------	------------------	-------------------	-------------------	-------------------	--------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Instrument was operating within Department of Health Regulations.

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JENNIFER A PERRY
---------------	-------------------------------------

TYPE II PERMIT NUMBER 250055	EXPIRATION DATE 02/20/2017	TELEPHONE NUMBER 573-882-7201
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901



Airgas USA LLC (LAB)
3500 Bernard Street
St. Louis, Mo. 63103
Ph: (314) 533-3100
Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 27-Oct-2014

Lot # AG429701

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
24-Oct-2016	108	Ethanol Nitrogen	0.080 ± 0.002 BrAC (208 ppm) Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
Date: 2014.10.27 10:15:24 -05:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Analyst: _____

Rod Marsala
Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

**PERMIT
 TYPE II**

JENNIFER PERRY

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):


DATAMASTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 2/20/2015

NUMBER 250055

EXPIRES 2/20/2017


 DIRECTOR OF STATE PUBLIC HEALTH LABORATORY


 ,acting director
 DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

 STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator PERRY, JENNIFER
 Permit No 250055
 Date Issued 2/20/2015 Date Expires 2/20/2017



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 901 Virginia Ave, Columbia		INSTRUMENT SERIAL NUMBER 500266	DATE OF TEST 07/04/2015	TIME OF TEST 04:56:12
SUBJECT NAME JENNIFER ANN PERRY			DATE OF BIRTH 09/23/1977	
SEX F	SUBJECT DRIVER'S LICENSE NUMBER M001242016		STATE MO	
ARRESTING OFFICER TEST TEST		ARRESTING OFFICER ID NA		
OPERATOR JENNIFER PERRY		OPERATOR PERMIT 250055	PERMIT EXP DATE 02/20/2017	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JENNIFER PERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	04:57
INTERNAL STANDARD	VERIFIED	04:57
SUBJECT SAMPLE (Vol=2.31L)	0.000	04:57
BLANK TEST	0.000	04:58

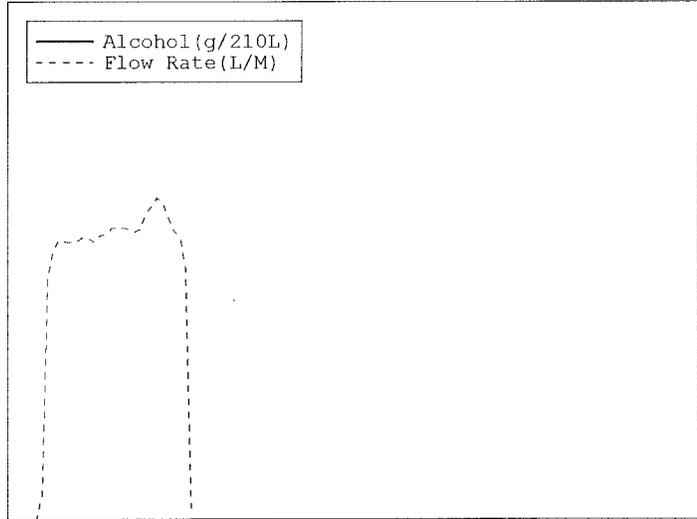

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR 	DATE 07/04/2015
WITNESS (IF ANY)	DATE 07/04/2015