

**RECEIVED**

By Ellen Strawsine at 10:47 am, Jan 21, 2016



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

REPORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 201211	NAME OF AGENCY Bella Villa P.D.	DATE OF INSPECTION 01/07/2016
LOCATION OF INSTRUMENT (STREET AND CITY) 751 Avenue H, Bella Villa, Mo 63125		TIME OF INSPECTION 2:58 am

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) <u>01/07/2016, 02:58 Hours</u>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER _____ 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

 INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER Guth LOT # 15120 EXP. DATE 04/29/2017

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN DR 2765 EXP. DATE 04/07/2016

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

- 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE  
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE  
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 → 0.99

TEST 2 → 0.100

TEST 3 → 0.100

 PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	0	(0-.04)	0	(.05-.09)	0	(.10-.14)	0	(.15-.19)	0	OVER .19	0
----------	---	---------	---	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

**INSPECTING OFFICER**

SIGNATURE

PRINT FULL NAME

Peter Palombo

TYPE II PERMIT NUMBER/EXPIRATION DATE

01/22/2016

TELEPHONE NUMBER

(314) 833-3340

RETURN COMPLETED REPORT TO THE:

Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office  
2875 James Blvd.  
Poplar Bluff, MO 63901



## GUTH LABORATORIES, INC.

590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-664-8470

### CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number 15120 of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on May 4, 2015, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain 0.1209% (w/vol) ethyl alcohol. The expiration date for this lot number is April 29, 2017 at 11:59 PM.

When used in a calibrated Simulator, operating at 34°C +/- 0.2°C, this solution will give a breath alcohol analysis instrument reading of 0.100 g/210L +/- 3%.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
GUTH LABORATORIES, INC.

**NIST Traceability:**

Testing was conducted using Cerilliant Reference Standard lot number FN03051301 whose values are traceable to NIST.

All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.



Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
BAC DATAMASTER SERIAL NUMBER 201211  
01/07/16

ARREST TIME: 00:00  
SUBJECT NAME:  
SOBER/TEST  
DOB: 11/11/11 SEX: M  
STATE/D.L.: MO/1111  
ARRESTING OFFICER:  
PALOMBO/P  
OFFICER I.D.: 38  
TESTING OFFICER:  
PALOMBO/P  
OFFICER I.D.: 38  
PERMIT NUMBER: 240177  
EXPIRATION DATE: 04/22/16  
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

BLANK TEST	.000	03:02
INTERNAL STANDARD	VERIFIED	03:03
SUBJECT SAMPLE	.000	03:08
BLANK TEST	.000	03:09

Signature 

2208-02

Face This Side Down - This Edge In First

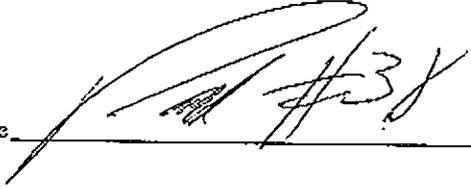
**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
BAC DATAMASTER SERIAL NUMBER 201211  
01/07/16

ARREST TIME: 00:00  
SUBJECT NAME:  
RADIO/TEST  
DOB: 11/11/11 SEX: M  
STATE/D.L.: MO/1111  
ARRESTING OFFICER:  
PALOMBO/P  
OFFICER I.D.: 38  
TESTING OFFICER:  
PALOMBO/P  
OFFICER I.D.: 38  
PERMIT NUMBER: 240177  
EXPIRATION DATE: 04/22/16  
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---

RADIO INTERFERENCE

Operator Signature 

2208-02



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*



Operator PALOMBO, PETER  
Permit No 240177  
Date Issued 4/22/2014 Date Expires 4/22/2016