



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
 INTOX DMT MAINTENANCE REPORT

**RECEIVED**

By Carol Day at 9:16 am, May 20, 2016

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500004	NAME OF AGENCY St. Louis County Police Department	DATE OF INSPECTION 05/17/2016
------------------------	--	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) South County Pct: 323 Sappington Barracks Rd.	TIME OF INSPECTION 01:45:40
---	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>05/17/2016 01:45:42</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG530301</u>	EXP. DATE <u>10/30/2017</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
--	--------------------	--------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.099	TEST 2: 0.099	TEST 3: 0.099
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST
---

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 2	0-.04: 0	.05-.09: 1	.10-.14: 3	.15-.19: 2	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE <i>Sgt D. R. [Signature]</i>	PRINT FULL NAME DONALD M JACQUIN
---	-------------------------------------

TYPE II PERMIT NUMBER 240392	EXPIRATION DATE 11/13/2016	TELEPHONE NUMBER 314-615-4266
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901



Airgas USA LLC (LAB)  
3600 Bernard Street  
St. Louis, Mo. 63103  
Ph: (314) 533-3100  
Fax: (314) 533-7328

## Certificate of Analysis

Customer Name  
Exclusive Supplier  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

Test Date: 30-Oct-2015

Lot # AG530301 Model 108cadd

<u>Exp. Date</u>	<u>Cvl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
30-Oct-2017	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm) Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

Analytical Method: NDIR

Digitally signed by Quality Control  
Date: 2015.10.30 15:34:04 -05:00  
Reason: Dry gas standard certification of analysts  
Location: Airgas USA LLC (Lab)

Analyst: \_\_\_\_\_

  
Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

2

**PERMIT**  
**TYPE II**

**DONALD M JACQUIN**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER, INTOX DMT**


for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 11/13/2014

NUMBER 240392

EXPIRES 11/13/2016

  
\_\_\_\_\_  
DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

  
\_\_\_\_\_  
,acting director  
DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

STANDARD CHANGE

-----  
St. Louis County Police Department  
INTOX dmt: 500004  
-----

Date: 05/17/2016  
Time: 01:42:22


OPERATOR NAME:  
DONALD M JACQUIN  
PERMIT NUMBER: 240392  
EXPIRATION DATE: 11/13/2016

LOT #: AG530301  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 10/30/2017  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.099

BLANK TEST	0.000	01:43
INTERNAL STANDARD	VERIFIED	01:43
EXTERNAL STANDARD	0.098	01:43
BLANK TEST	0.000	01:44

Average = 0.0980  
Std Dev = 0.0000  
Spread = 0.0000

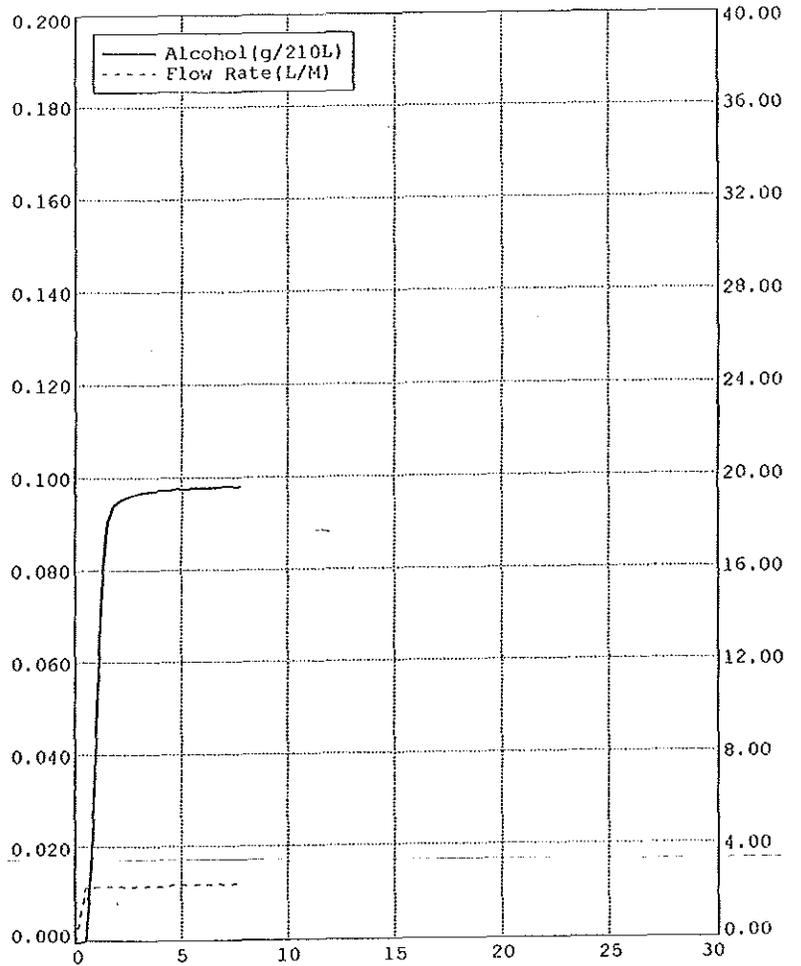

Sgt D JF 3056