

RECEIVED

By Carol Day at 8:41 am, Apr 25, 2016



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500042	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 04/14/2016
------------------------	---	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 2920 N. Shamrock, Jefferson City, MO	TIME OF INSPECTION 14:46:01
--	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>04/14/2016 14:46:03</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG604101</u>	EXP. DATE <u>02/10/2018</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
--	--------------------	--------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.099	TEST 2: 0.099	TEST 3: 0.099
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Instrument calibrated and standard change performed. Dry Gas regulator assembly replaced.

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JIMMY L CLEVELAND
---------------	--------------------------------------

TYPE II PERMIT NUMBER 250155	EXPIRATION DATE 07/22/2017	TELEPHONE NUMBER 573-526-6193
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901

CALIBRATION FACTORS


Missouri State Highway Patrol
INTOX dmt: 500042

Date: 04/07/2016
Time: 09:02:20

OPERATOR NAME:
JIMMY L CLEVELAND
PERMIT NUMBER: 250155
EXPIRATION DATE: 07/22/2017
MISC:
GUTH 12V500 SER MP2316 EXP 031517

LOT #: 14001
SUPPLIER: REPCO
EXPIRATION: 04/30/2016

Ca	=	0.1000			
ADJ	=	1.022219	0.800	<=	ADJ < 1.200
b1	=	0.0004	0.0000	<=	b1 < 0.0040
b2	=	0.0047	0.0010	<=	b2 < 0.0100
b3	=	0.0005	0.0000	<=	b3 < 0.0040
Xq	=	0.0992	0.0500	<=	Xq < 0.2500
a21	=	1.147103	1.050	<=	a21 < 1.300
a31	=	0.569066	0.300	<=	a31 < 0.800

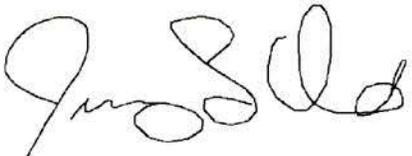

STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500042

Date: 04/12/2016
Time: 14:16:13


OPERATOR NAME:
JIMMY L CLEVELAND
PERMIT NUMBER: 250155
EXPIRATION DATE: 07/22/2017

LOT #: AG604101
SUPPLIER: INTOXIMETERS
EXPIRATION: 02/10/2018
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.098

BLANK TEST	0.000	14:17
INTERNAL STANDARD	VERIFIED	14:17
EXTERNAL STANDARD	0.100	14:17
BLANK TEST	0.000	14:18

Average = 0.1000
Std Dev = 0.0000
Spread = 0.0000

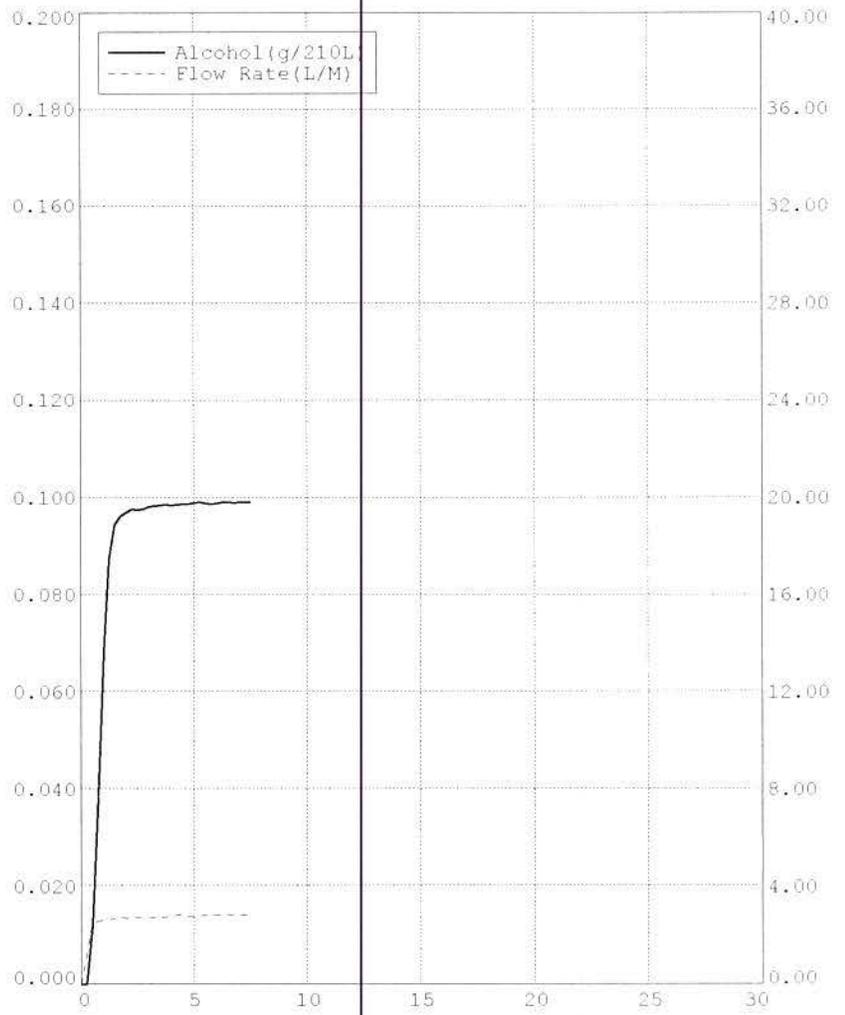

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.

LOT NUMBER: 14001

EXPIRATION DATE: April 30, 2016 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 14001 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1216 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% gms/210L Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is May 1, 2014
The expiration date for this lot number is April 30, 2016 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 13-Feb-2016

Lot # AG604101 Model 108cacd

Exp. Date

10-Feb-2018

Cyl. Type

108

Component

Ethanol
Nitrogen

Certified Concentration

0.100 ± 2% BrAC (260 ppm)
Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

Serial No.

EB0010581
EB0010570
EB0010285
EB0010561
EB0010681

Concentration

391.8 ppm
259.8 ppm
209.0 ppm
103.7 ppm
52.22 ppm

Serial No.

EB0010603
EB0010559
EB0010595
EB0010562
EB0010579

Concentration

392.5 ppm
258.9 ppm
208.9 ppm
104.9 ppm
52.94 ppm

Analytical Method:

NDIR

Digitally signed by Quality Control
Date: 2016.02.15 09:32:28 -06:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Analyst: _____

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

**PERMIT
 TYPE II**

JIMMY L CLEVELAND

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

ALCO-SENSOR IV WITH PRINTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 7/22/2015

NUMBER 250155

EXPIRES 7/22/2017

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R5-10)



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator CLEVELAND, JIMMY
 Permit No 250155
 Date Issued 7/22/2015 Date Expires 7/22/2017