



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500046	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 07/29/2016
LOCATION OF INSTRUMENT (STREET AND CITY) 10 N.E. Tudor Road., Lee's Summit		TIME OF INSPECTION 09:13:56

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>07/29/2016 09:13:59</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.6°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER AIRGAS LOT # AG615304 EXP. DATE 06/01/2018

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.101 TEST 2: 0.101 TEST 3: 0.101

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 1	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

CHANGED OUT DRY GAS CANISTER. NEW CANISTER CONTAINS 0.100+/- 2% BRAC CONCENTRATION. CANISTER EXPIRES 06/01/2018.

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME DANIEL D WOHLER
---------------	---

TYPE II PERMIT NUMBER 250317	EXPIRATION DATE 12/28/2017	TELEPHONE NUMBER 816-622-0800
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901

STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500046

Date: 07/29/2016
Time: 09:10:11


OPERATOR NAME:
DANIEL D WOHLER
PERMIT NUMBER: 250317
EXPIRATION DATE: 12/28/2017

LOT #: AG615304
SUPPLIER: AIRGAS
EXPIRATION: 06/01/2018
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.096

BLANK TEST	0.000	09:11
INTERNAL STANDARD	VERIFIED	09:11
EXTERNAL STANDARD	0.097	09:11
BLANK TEST	0.000	09:12

Average = 0.0970
Std Dev = 0.0000
Spread = 0.0000

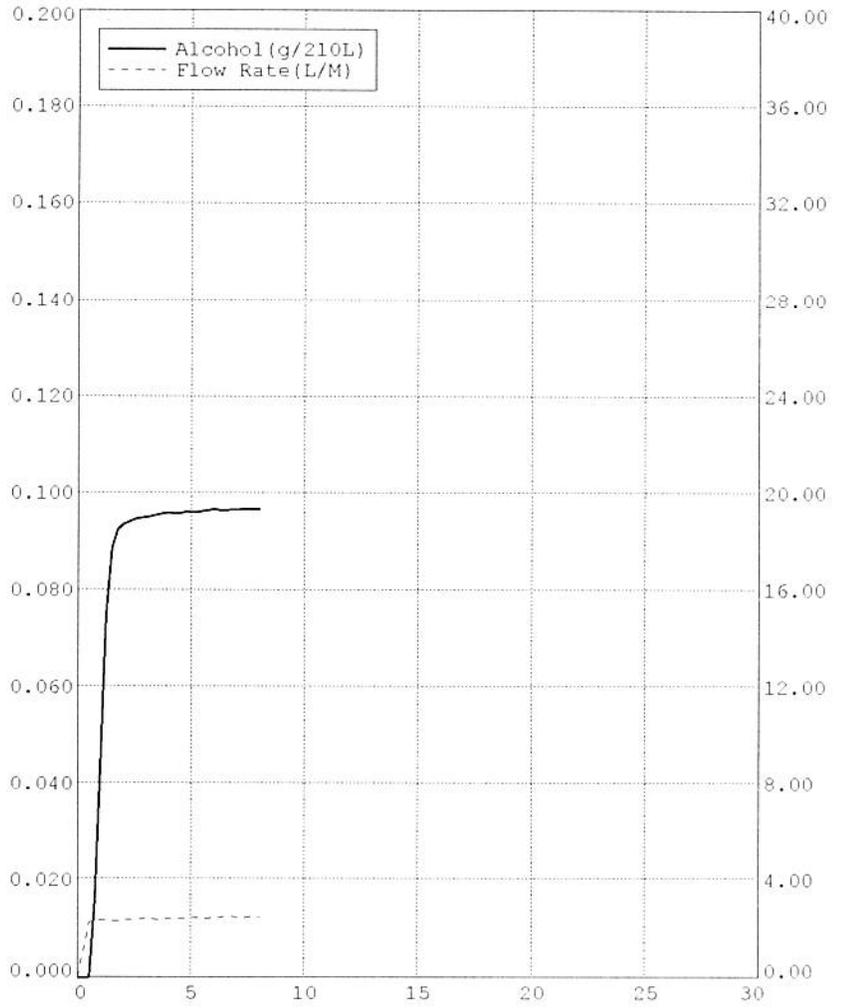

[Handwritten Signature] #1354



Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Customer Name
 Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 2-Jun-2016

Lot # AG615304 Model 108cacc

Exp. Date 1-Jun-2018	Cyl. Type 108	Component Ethanol Nitrogen	Certified Concentration 0.100 ± 2% BrAC (260 ppm) Balance
--------------------------------	-------------------------	---	--

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
 Date: 2016.06.02 13:08:52 -05:00
 Reason: Dry gas standard certification of analysis
 Location: Airgas USA LLC (Lab)

Analyst: 
 Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 10 N.E. Tudor Road., Lee's Summit		INSTRUMENT SERIAL NUMBER 500046	DATE OF TEST 07/29/2016	TIME OF TEST 09:23:16
SUBJECT NAME SELF TEST			DATE OF BIRTH 01/01/2001	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER 123456		STATE MO	
ARRESTING OFFICER DANIEL D WOHLER		ARRESTING OFFICER ID 1394		
OPERATOR DANIEL WOHLER		OPERATOR PERMIT 250317	PERMIT EXP DATE 12/28/2017	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by DANIEL WOHLER. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	09:24
INTERNAL STANDARD	VERIFIED	09:24
SUBJECT SAMPLE (Vol=1.69L)	0.000	09:24
BLANK TEST	0.000	09:25

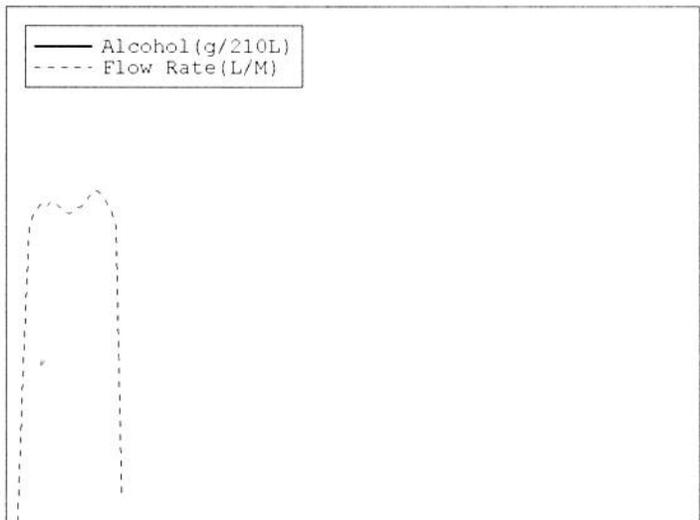

COMMENTS

SELF TEST AFTER STADARD CHANGE AND MAINTENANCE REPORT

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

Daniel Wohler

DATE
07/29/2016

WITNESS (IF ANY)

DATE



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

2

**PERMIT
TYPE II**

DANIEL WOHLER

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 12/28/2015

NUMBER 250317

EXPIRES 12/28/2017

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-07/1 (6-10)

LAB-4 (R5-10)

STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator **WOHLER, DANIEL**
Permit No **250317**
Date Issued **12/28/2015** Date Expires **12/28/2017**