



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

**RECEIVED**  
 By Carol Day at 11:50 am, May 18, 2016

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days)  
 Complete this report whenever the instrument is serviced or repaired and when a new instrument is placed into service  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN <b>500111</b>	NAME OF AGENCY <b>Missouri State Highway Patrol</b>	DATE OF INSPECTION <b>05/18/2016</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>211 South New Madrid, Benton, Missouri</b>		TIME OF INSPECTION <b>08:52:10</b>

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>05/18/2016 08:52:12</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.6°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

SIMULATOR STANDARD       COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER AIRGAS      LOT # AG516802      EXP. DATE 06/17/2017

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_      SIMULATOR SN \_\_\_\_\_      SIMULATOR EXP DATE \_\_\_\_\_

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.099      TEST 2: 0.099      TEST 3: 0.099

**PERFORM R.F.I. TEST**

**INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:**

REFUSALS: 1	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME <b>ANDREW F CHEANEY</b>
---------------	--

TYPE II PERMIT NUMBER <b>260013</b>	EXPIRATION DATE <b>01/14/2018</b>	TELEPHONE NUMBER <b>573-840-9500</b>
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901





STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

2

**PERMIT**  
**TYPE II**  
**ANDREW F CHEANEY**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 1/14/2016

NUMBER 260013

EXPIRES 1/14/2018

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES



**STATE OF MISSOURI**  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*



Operator CHEANEY, ANDREW  
Permit No 260013  
Date Issued 1/14/2016 Date Expires 1/14/2018

STANDARD CHANGE

-----  
Missouri State Highway Patrol  
INTOX dmt: 500111  
-----

Date: 05/18/2016  
Time: 08:48:02


OPERATOR NAME:  
ANDREW F CHEANEY  
PERMIT NUMBER: 260013  
EXPIRATION DATE: 01/14/2018

LOT #: AG516802  
SUPPLIER: AIRGAS  
EXPIRATION: 06/17/2017  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.099

BLANK TEST	0.000	08:49
INTERNAL STANDARD	VERIFIED	08:49
EXTERNAL STANDARD	0.102	08:49
BLANK TEST	0.000	08:50

Average = 0.1020  
Std Dev = 0.0000  
Spread = 0.0000

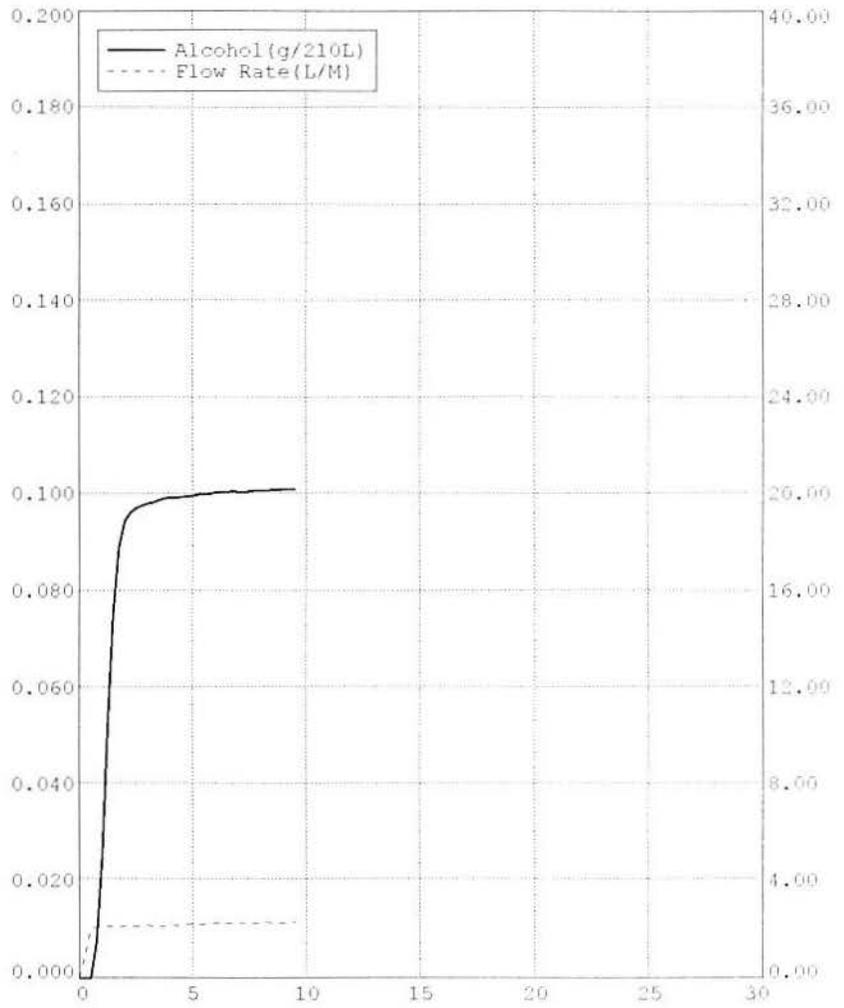

AC