





Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**

*Exclusive Supplier*  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 2-Jun-2016

**Lot # AG615304 Model 108caccd**

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
1-Jun-2018	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm) Balance

**Certification Traceable to N.I.S.T. RGM Ethanol Standards:**

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

**Analytical Method:** NDIR

Digitally signed by Quality Control  
Date: 2016.06.02 13:08:52 -05:00  
Reason: Dry gas standard certification of analysis  
Location: Airgas USA LLC (Lab)

Analyst: \_\_\_\_\_

Rod Marsala

**ISO 17025:2005 A2LA accredited. Certificate Number 2989.01**

STANDARD CHANGE

-----  
Missouri State Highway Patrol  
INTOX dmt: 500150  
-----

Date: 06/27/2016  
Time: 13:03:23


OPERATOR NAME:  
JIMMY L CLEVELAND  
PERMIT NUMBER: 250155  
EXPIRATION DATE: 07/22/2017

LOT #: AG615304  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 06/01/2018  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.098

BLANK TEST	0.000	13:04
INTERNAL STANDARD	VERIFIED	13:04
EXTERNAL STANDARD	0.096	13:04
BLANK TEST	0.000	13:05

Average = 0.0960  
Std Dev = 0.0000  
Spread = 0.0000

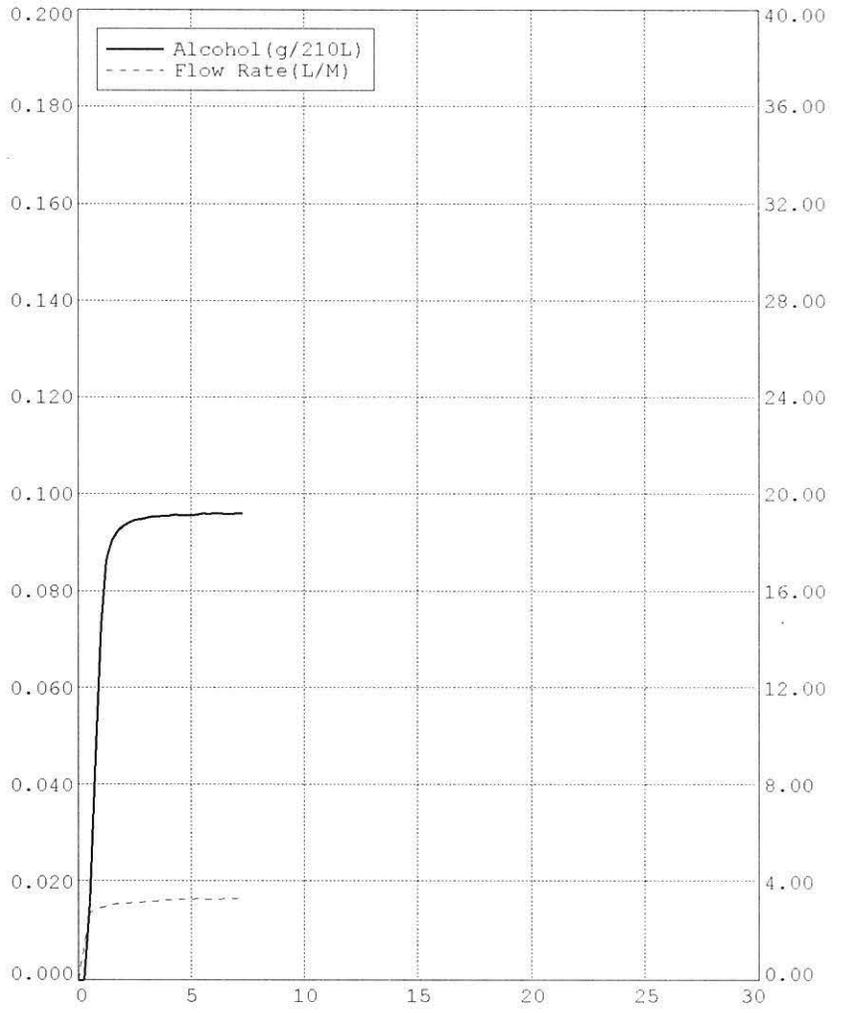

*9200*



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

2

**PERMIT  
 TYPE II**

**JIMMY L CLEVELAND**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**ALCO-SENSOR IV WITH PRINTER, INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 7/22/2015

NUMBER 250155

EXPIRES 7/22/2017

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 582-0/71 (6 10)

LAB-4 (R5-10)



**STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*



Operator CLEVELAND, JIMMY  
 Permit No 250155  
 Date Issued 7/22/2015 Date Expires 7/22/2017