



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500204	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 05/12/2016
LOCATION OF INSTRUMENT (STREET AND CITY) 2920 N. Shamrock, Jefferson City		TIME OF INSPECTION 14:02:40

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>05/12/2016 14:02:42</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.7°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG604101 EXP. DATE 02/10/2018

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.101 TEST 2: 0.100 TEST 3: 0.100

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Instrument calibrated and standard change performed. Bias Voltage and Chopper setting adjusted

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JIMMY L CLEVELAND
TYPE II PERMIT NUMBER 250155	EXPIRATION DATE 07/22/2017
	TELEPHONE NUMBER 573-526-6193

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901

CALIBRATION FACTORS

Missouri State Highway Patrol
INTOX dmt: 500204

Date: 05/12/2016
Time: 09:10:26

OPERATOR NAME:
JIMMY L CLEVELAND
PERMIT NUMBER: 250155
EXPIRATION DATE: 07/22/2017
MISC:
GUTH 12V500 SER MP2316 EXP 031517

LOT #: 15001
SUPPLIER: REPCO
EXPIRATION: 05/20/2017

Ca = 0.1000
ADJ = 1.018840 0.800 <= ADJ < 1.200
b1 = 0.0015 0.0000 <= b1 < 0.0040
b2 = 0.0057 0.0010 <= b2 < 0.0100
b3 = 0.0011 0.0000 <= b3 < 0.0040
Xq = 0.0855 0.0500 <= Xq < 0.2500
a21 = 1.124650 1.050 <= a21 < 1.300
a31 = 0.501654 0.300 <= a31 < 0.800



STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500204

Date: 05/11/2016
Time: 13:35:21


OPERATOR NAME:
JIMMY L CLEVELAND
PERMIT NUMBER: 250155
EXPIRATION DATE: 07/22/2017

LOT #: AG604101
SUPPLIER: INTOXIMETERS
EXPIRATION: 02/10/2018
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.097

BLANK TEST	0.000	13:36
INTERNAL STANDARD	VERIFIED	13:36
EXTERNAL STANDARD	0.099	13:36
BLANK TEST	0.000	13:37

Average = 0.0990
Std Dev = 0.0000
Spread = 0.0000

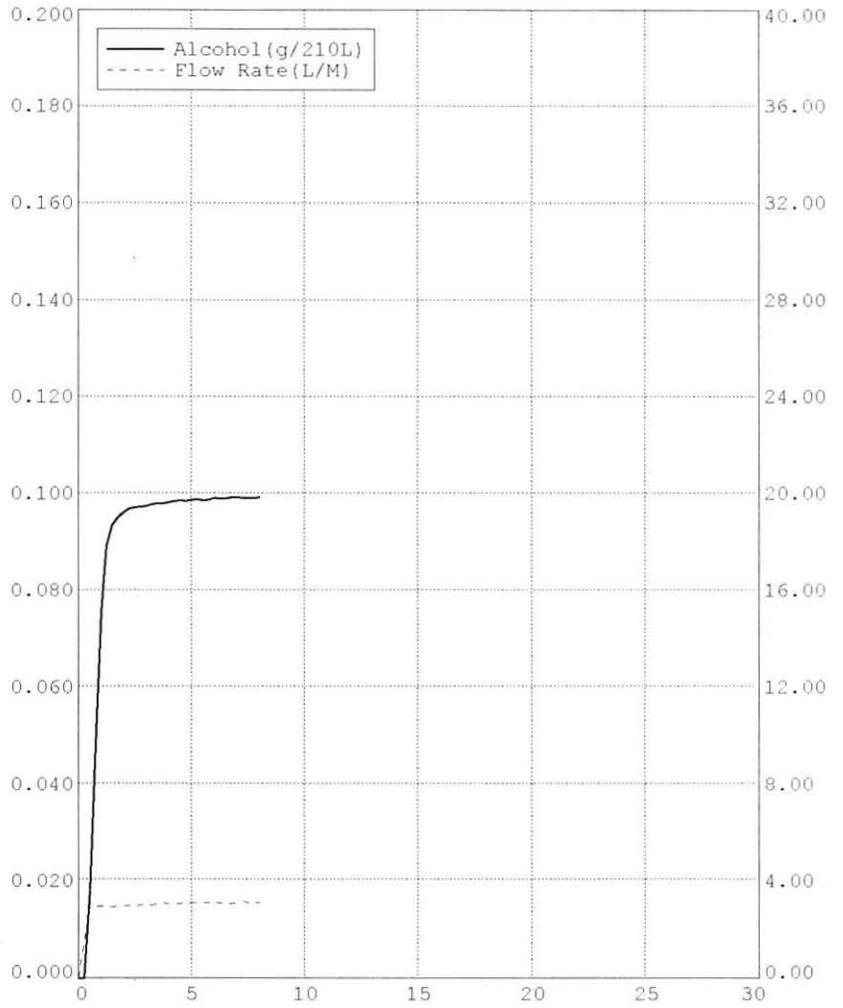



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 13-Feb-2016

Lot # AG604101 Model 108cacd

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
10-Feb-2018	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm) Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
Date: 2016.02.15 09:32:28 -06:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Analyst: _____

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01

REPCO MARKETING INC.3101-188 STONYBROOK DRIVE
RALEIGH, N.C. 27604
919-876-5480**CERTIFICATE OF ANALYSIS****MANUFACTURER AND SUPPLIER: RepCo Marketing, Inc.****LOT NUMBER: 15001****EXPIRATION DATE: May 20, 2017 at 11:59 p.m.**

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 15001 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1206 gms/dl +/-0.003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/-3% gms/210L Breath when heated to 34 Degrees Celsius +/-0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is May 21, 2015
The expiration date for this lot number is May 20, 2017 at
11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President
RepCo Marketing, Inc.



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM



**PERMIT
TYPE II**

JIMMY L CLEVELAND

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

ALCO-SENSOR IV WITH PRINTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 7/22/2015

NUMBER 250155

EXPIRES 7/22/2017

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-9/71 (6 10)

LAB-4 (R5-10)



STATE OF MISSOURI
DEPARTMENT OF HEALTH AND SENIOR SERVICES
BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.



Operator CLEVELAND, JIMMY
Permit No 250155
Date Issued 7/22/2015 Date Expires 7/22/2017