



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN <b>500252</b>	NAME OF AGENCY <b>Cameron Police Department</b>	DATE OF INSPECTION <b>04/01/2016</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>101 North Chestnut, Cameron, Missouri 64429</b>		TIME OF INSPECTION <b>02:10:40</b>

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>04/01/2016 02:10:42</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.6°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG511702</u> EXP. DATE <u>04/27/2017</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____ SIMULATOR EXP DATE _____

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.076	TEST 2: 0.077	TEST 3: 0.076
<input checked="" type="checkbox"/> PERFORM R.F.I. TEST		

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:					
REFUSALS: 1	0-.04: 1	.05-.09: 0	.10-.14: 1	.15-.19: 1	OVER .19: 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

<b>INSPECTING OFFICER</b>			
SIGNATURE <i>Shane T Stevenson</i>	PRINT FULL NAME <b>SHANE T STEVENSON</b>		
TYPE II PERMIT NUMBER <b>250075</b>	EXPIRATION DATE <b>03/31/2017</b>	TELEPHONE NUMBER <b>816-632-2177</b>	

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
Southeast District Office  
2875 James Blvd, Poplar Bluff, MO 63901



Airgas USA LLC (LAB)  
3500 Bernard Street  
St. Louis, Mo. 63103  
Ph: (314) 533-3100  
Fax: (314) 533-7328

## Certificate of Analysis

Customer Name  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

Test Date: 28-Apr-2015

Lot # AG511702

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
27-Apr-2017	108	Ethanol	0.080 ± 0.002 BrAC (208.4 ppm)
		Nitrogen	Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

Analytical Method: NDIR

Digitally signed by Quality Control  
Date: 2015.04.29 13:39:10 -05:00  
Reason: Dry gas standard certification of analysis  
Location: Airgas USA LLC (Lab)

Analyst: \_\_\_\_\_

Yusef Woods

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

2

**PERMIT  
TYPE II**

**SHANE T STEVENSON**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 3/31/2015

NUMBER 250075

EXPIRES 3/31/2017

KID 650-0771 (5-12)

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (RS-10)



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*



Operator STEVENSON, SHANE  
Permit No 250075  
Date Issued 3/31/2015 Date Expires 3/31/2017



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 101 North Chestnut, Cameron, Missouri 64429		INSTRUMENT SERIAL NUMBER 500252	DATE OF TEST 04/01/2016	TIME OF TEST 02:20:31
SUBJECT NAME SHANE T STEVENSON			DATE OF BIRTH 12/20/1973	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER T980647589		STATE MO	
ARRESTING OFFICER SHANE T STEVENSON		ARRESTING OFFICER ID 110		
OPERATOR SHANE T STEVENSON		OPERATOR PERMIT 250075	PERMIT EXP DATE 03/31/2017	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by SHANE T STEVENSON. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	02:21
INTERNAL STANDARD	VERIFIED	02:21
SUBJECT SAMPLE (Vol=3.04L)	0.000	02:22
BLANK TEST	0.000	02:23

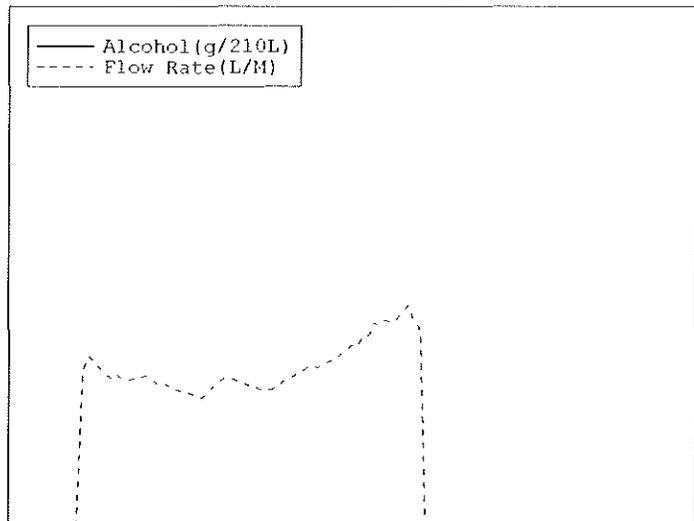

COMMENTS

CERTIFICATION BY OPERATOR

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR <i>Shane T Stevenson #110</i>	DATE 04/01/2016
WITNESS (IF ANY)	DATE 04/01/2016