



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM

**RECEIVED**  
 By Carol Day at 10:09 am, Mar 03, 2016

**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN <b>500276</b>	NAME OF AGENCY <b>St. Louis County Police Department</b>	DATE OF INSPECTION <b>03/02/2016</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>Jennings Precinct - 5445 Jennings Station Rd 63136</b>		TIME OF INSPECTION <b>12:36:02</b>

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>03/02/2016 12:36:04</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>46.5°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

SIMULATOR STANDARD       COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS      LOT # AG418902      EXP. DATE 07/08/2016

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_      SIMULATOR SN \_\_\_\_\_      SIMULATOR EXP DATE \_\_\_\_\_

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: **0.099**      TEST 2: **0.099**      TEST 3: **0.099**

**PERFORM R.F.I. TEST**

**INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:**

REFUSALS: <b>0</b>	0-.04: <b>1</b>	.05-.09: <b>2</b>	.10-.14: <b>3</b>	.15-.19: <b>0</b>	OVER .19: <b>1</b>
--------------------	-----------------	-------------------	-------------------	-------------------	--------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE <i>Det. Stoechner 3732</i>	PRINT FULL NAME <b>DET STOECHNER</b>
TYPE II PERMIT NUMBER <b>250236</b>	TELEPHONE NUMBER <b>636-529-8210</b>

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901**



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
**BLOOD ALCOHOL TEST REPORT - INTOX DMT**

FORM #11


LOCATION OF INSTRUMENT Jennings Precinct - 5445 Jennings Station Rd 63136		INSTRUMENT SERIAL NUMBER 500276	DATE OF TEST 03/02/2016	TIME OF TEST 12:45:01
SUBJECT NAME SOBER TEST			DATE OF BIRTH 01/01/2001	
SEX F	SUBJECT DRIVER'S LICENSE NUMBER NA		STATE MO	
ARRESTING OFFICER DET STOEHNER		ARRESTING OFFICER ID 3932		
OPERATOR DET STOEHNER		OPERATOR PERMIT 250236	PERMIT EXP DATE 10/30/2017	

**OPERATIONAL CHECKLIST: INTOX DMT**

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by DET STOEHNER. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

**SUBJECT TEST RESULTS**

BLANK TEST	0.000	12:45
INTERNAL STANDARD	VERIFIED	12:46
SUBJECT SAMPLE (Vol=2.10L)	0.000	12:46
BLANK TEST	0.000	12:47

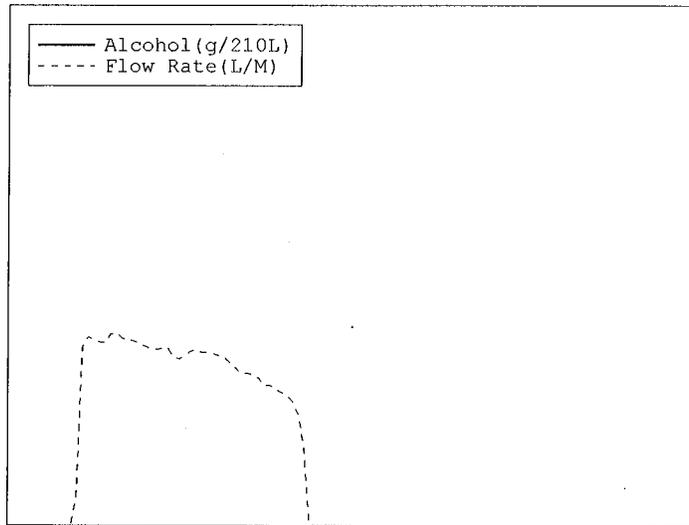

COMMENTS

**CERTIFICATION BY OPERATOR**

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR *Det Stoenner-3932* DATE 03/02/2016

WITNESS (IF ANY) DATE 03/02/2016



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

2

**PERMIT  
 TYPE II**

**STEPHANIE M STOEHNER**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**DATAMASTER, INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 10/30/2015

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

NUMBER 250236

EXPIRES 10/30/2017

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

 **STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*



Operator **STOEHNER, STEPHANIE**  
 Permit No **250236**  
 Date issued **10/30/2015** Date Expires **10/30/2017**



Airgas USA LLC (LAB)  
 3500 Bernard Street  
 St. Louis, Mo. 63103  
 Ph: (314) 533-3100  
 Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**  
 Intoximeters, Inc.  
 2081 Craig Road  
 St. Louis, Mo 63146

**Test Date:** 8-Jul-2014

**Lot # AG418902**


<b>Exp. Date</b> 8-Jul-2016	<b>Cyl. Type</b> 108	<b>Component</b> Ethanol Nitrogen	<b>Certified Concentration</b> 0.100 ± 2% BrAC (260 ppm) Balance
--------------------------------	-------------------------	---	--

**Certification Traceable to N.I.S.T. RGM Ethanol Standards:**

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm.	EB0010595	208.9 ppm
EB0010561	103.7 ppm	EB0010562	104.9 ppm
EB0010681	52.22 ppm	EB0010579	52.94 ppm

**Analytical Method:** NDIR

Digitally signed by Quality Control  
 Date: 2014.07.08 16:23:57 -05:00  
 Reason: Dry gas standard certification of analysis  
 Location: Airgas USA LLC (Lab)

**Analyst:**   
 Rod Marsala

**ISO 17025:2005 A2LA accredited. Certificate Number 2989.01**