



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
DATAMASTER MAINTENANCE REPORT

REPORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER SN 950117	NAME OF AGENCY Brookfield Police Dept.	DATE OF INSPECTION 02/07/2016
-------------------------	---	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 116. W. Brooks St. Brookfield, MO 64628	TIME OF INSPECTION 2:40 pm
---	-------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) <u>02-07-16 14:40</u>
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER <u>50</u> °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

INDICATOR LIGHTS

SIMULATOR SOLUTION SUPPLIER RepCo Marketing Inc. LOT # 14001 EXP. DATE 04/30/2016

SIMULATOR TEMP (34°C ± 0.2°C) 34.0 °C SIMULATOR SN SD2763 EXP. DATE 03/05/2016

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

- 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 <u>.100</u>	TEST 2 <u>.100</u>	TEST 3 <u>.100</u>
--------------------	--------------------	--------------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
(DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	0	(0-.04)	15	(.05-.09)	0	(.10-.14)	0	(.15-.19)	0	OVER .19	0
----------	---	---------	----	-----------	---	-----------	---	-----------	---	----------	---

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME Stuart Hughes
---------------	----------------------------------

TYPE II PERM NUMBER/EXPIRATION DATE 260015 / 01/05/2018	TELEPHONE NUMBER (660) 258-3385
--	------------------------------------

RETURN COMPLETED REPORT TO THE:
Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office
2875 James Blvd.
Poplar Bluff, MO 63901


BAC DataMaster
Evidence Ticket

STATE OF MISSOURI
BAC DATA MASTER SERIAL NUMBER 959117
02/07/16
14:43

--- DIAGNOSTIC CHECK ---

COMPACT	OKAY
PROPERM (04-97-0000)	OKAY
PROPERM	OKAY
PROPERM (04-97-0000)	OKAY
PROPERM	OKAY
PROPERM (04-97-0000)	OKAY
PROPERM	OKAY
PROPERM (04-97-0000)	OKAY
PROPERM	OKAY
PROPERM (04-97-0000)	OKAY
PROPERM	OKAY
PROPERM (04-97-0000)	OKAY
PROPERM	OKAY

SEMI-ANNUAL TEST
16602587279 (16602587279) (16602587279)
16602587279 (16602587279) (16602587279)
16602587279 (16602587279) (16602587279)

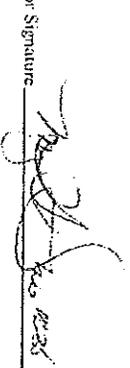Officer Signature 

BAC DataMaster
Evidence Ticket

STATE OF MISSOURI
BAC DATA MASTER SERIAL NUMBER 959117
02/07/16

TESTING OFFICER:

PLUMMER/STUART
OFFICER I.D.: 235
PERMIT NUMBER: 260015
EXPIRATION DATE: 01/05/18
MISCELLANEOUS DATA:

--- SUPERVISOR NODE ---

BLANK TEST	.000	14:43
INTERNAL STANDARD	.100	14:43
EXTERNAL STANDARD	.100	14:44
BLANK TEST	.000	14:44
EXTERNAL STANDARD	.100	14:45
BLANK TEST	.000	14:45
EXTERNAL STANDARD	.100	14:46
BLANK TEST	.000	14:47

N = 3
SIN. = .1
AVG. = .1

Officer Signature 

BAC DataMaster
Evidence Ticket

STATE OF MISSOURI
BAC DATA MASTER SERIAL NUMBER 95911
02/07/16

ARREST TIME: 14:23


SUBJECT NAME:
SUSPECTOR
DOB: 12/28/90 SEX: M
STATE/D.L.: MO/122/34-5678
ARRESTING OFFICER:
PLUMMER/STUART
OFFICER I.D.: 235
TESTING OFFICER:
SPME

OFFICER I.D.: 235
PERMIT NUMBER: 260015
EXPIRATION DATE: 01/05/18
MISCELLANEOUS DATA:

--- BREATH ANALYSIS ---


BLANK TEST	.000	1
INTERNAL STANDARD	.100	1
RADIO INTERFERENCE	.000	1

Officer Signature 

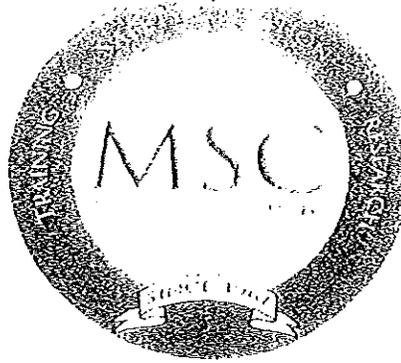

Simulator Calibration Report

This calibration report is to certify the alcohol reference simulator listed below has been examined and tested using standards traceable to the National Institute of Standards and Technology (NIST) in accordance with the standards set by the Missouri Department of Health and Senior Services Rules and Regulations 19 CSR 25-30.051 (4).

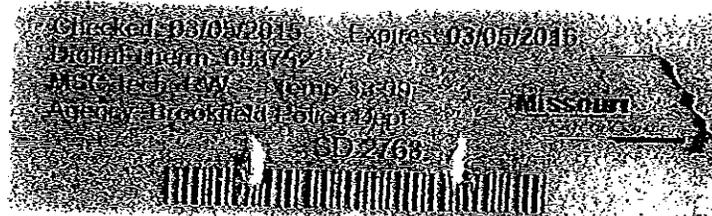

Technician Printed Name: ROBERT WELSH

Technician Signature: *Robert Welsh*

Date: 03/05/2015

Contact: Missouri Safety Center
Breath-Alcohol Instrument Training Program
660-543-4834

CERTIFICATE OF ANALYSIS

MANUFACTURER AND SUPPLIER RepCo Marketing, Inc
LOT NUMBER: 14001
EXPIRATION DATE: April 30, 2016 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:


RepCo Marketing, Inc. manufactured, tested and supplied 14001 of Alcohol Certified Solution for simulators. Random samples number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1216 gms/dl +/- .003 gms/dl wt/vol eth (95% Confidence).

The alcohol and distilled water used in the solution were found to contain no interfering substance.

This solution will produce a vapor alcohol value of .100 +/- 3% Breath when heated to 34 Degrees Celsius +/- 0.2 Degrees Celsius in a (95% Confidence).

The date of manufacture for this lot number is May
The expiration date for this lot number is April 30, 2016
11:59 p.m.

This document is a true representation of the original Certificate of

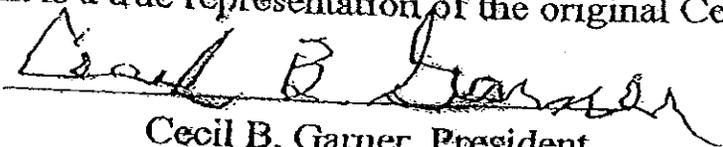

Cecil B. Garner, President
RepCo Marketing, Inc.