



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
ALCO-SENSOR IV WITH PRINTER MAINTENANCE REPORT

REPORT #7

Complete this report in duplicate at the time of the regular monthly preventative maintenance check, and whenever instrument is repaired. Send copy to Department of Health and Senior Services; retain original in department file.

ALCO SENSOR IV SN 102455	NAME OF AGENCY PETTIS CO SHERIFF'S OFFICE	DATE OF INSPECTION 08/24/2023
LOCATION OF INSTRUMENT (STREET AND CITY) 319 S LAMINE AVE, SEDALIA		TIME OF INSPECTION 2:09 am

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determined.) Unmarked items must be corrected before using instrument.

- DIGITAL READOUT (ALL ELEMENTS OPERATIONAL)
- TEMPERATURE OF ALCO SENSOR (10°C - 40°C)
- PRINTER WORKING PROPERLY
- TIME AND DATE DISPLAYING PROPERLY

BREATH ALCOHOL ACCURACY STANDARDS

- SIMULATOR SOLUTION COMPRESSED ETHANOL-GAS MIXTURE
- STANDARD SUPPLIER INTOXIMETERS LOT # AG110402 EXP. DATE 04/14/2023
- SIMULATOR TEMPERATURE (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

- CALIBRATION CHECK -- (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Check the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)
 - 0.100% STANDARD - MUST READ BETWEEN 0.095% and 0.105% INCLUSIVE
 - 0.080% STANDARD - MUST READ BETWEEN 0.076% and 0.084% INCLUSIVE
 - 0.040% STANDARD - MUST READ BETWEEN 0.038% and 0.042% INCLUSIVE

TEST 1 .080	TEST 2 .080	TEST 3 .080
--------------	--------------	--------------

- RFI DETECTOR OPERATING

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS	(0-.04)	(.05-.09)	(.10-.14)	(.15-.19)	(OVER .19)
----------	---------	-----------	-----------	-----------	------------

List any new parts and describe any alteration or modification that was made to restore the instrument to operate satisfactorily and within established limits (use other side if necessary).

Instrument operating within standards established by MODHSS

INSPECTING OFFICER	
SIGNATURE 	PRINT NAME Jimmy Moore
TYPE II PERMIT NUMBER/EXPIRATION DATE 210261 11/18/2023	TELEPHONE NUMBER (660) 827-0052

Return completed report to the: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office by mail, fax, or email.

AS IV Serial no: 102455
Version no: 532B

TEST RECORD 00286 %/
Temp Date Time 210L

Air Blank: 08/24/23 02:30 .000
Calibration Check: 21 08/24/23 02:30 .000

Subject Name Jimmy Moore
Subject I.D. 210261
Operator Name, I.D. 319S Lamine
Location Sedalia, MO

Test 2

AS IV Serial no: 102455
Version no: 532B

TEST RECORD 00287 %/
Temp Date Time 210L

Air Blank: 08/24/23 02:32 .000
Calibration Check: 22 08/24/23 02:32 .000

Subject Name Jimmy Moore
Subject I.D. 210261
Operator Name, I.D. 319 S Lamine
Location Sedalia MO

TEST 3

AS IV Serial no: 102455
Version no: 532B


TEST RECORD 00288 %/
Temp Date Time 210L

VOID: RFI
12 08/24/23 02:33

Subject Name Jimmy Moore
Subject I.D. 210261
Operator Name, I.D. 319 S. Lamine
Location Sedalia, MO

RFI


STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator **MOORE, JIMMY**
 Permit No **210261**
 Date Issued **11/18/2021** Date Expires **11/18/2023**



LAB 4 (R6:10)

MI0 580-0771 (6-10)

EXPIRES **11/18/2023**

NUMBER **210261**

DATE **11/18/2021**

 DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

 DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

ALCO-SENSOR IV WITH PRINTER, INTOX DMT


is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service, and repairs, and operate the following breath analyzer(s):

JIMMY D. MOORE

PERMIT
TYPE II

STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



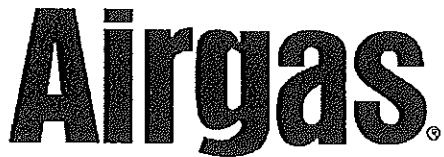

Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 533-7328

Certificate of Analysis

Customer Name
Exclusive Supplier
 Intoximeters, Inc.
 2081 Craig Road
 St. Louis, Mo 63146

Test Date: 20-Jul-2023

Lot # AG320005 **Model** 108

Exp Date 19-Jul-2025	Cyl. Type 108	Component Ethanol Nitrogen	Certified Concentration 0.080 ± 0.002 BrAC (218 ppm)
--------------------------------	-------------------------	---	--

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

Analytical Method: NDIR

Digitally signed by:Quality Control
 Reason:Dry gas standard certification of analysis
 Location:Airgas USA LLC (Lab)
 Date:07.20.2023 18:15

Approved for Release: _____

Rod Marsala

ISO 17025:2017 A2LA accredited. Certificate Number 3082.06
ISO 17034:2016 A2LA accredited. Certificate Number 3082.07