



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500016	NAME OF AGENCY Higginville Police Department	DATE OF INSPECTION 08/14/2023
LOCATION OF INSTRUMENT (STREET AND CITY) 12 W 19th Street, Higginville, MO		TIME OF INSPECTION 15:12:58

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>08/14/2023 15:13:00</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.6°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG208102 EXP. DATE 03/22/2024

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.099	TEST 2: 0.098	TEST 3: 0.098
----------------------	----------------------	----------------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0- .04: 0	.05-.09: 1	.10-.14: 0	.15-.19: 0	OVER .19: 0
--------------------	------------------	-------------------	-------------------	-------------------	--------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME QUINTON L DINOVI	
TYPE II PERMIZ NUMBER 210224	EXPIRATION DATE 10/05/2023	TELEPHONE NUMBER 660-584-2104

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email

STANDARD CHANGE

Higginsville Police Department
INTOX dmt: 500016

Date: 08/14/2023
Time: 15:09:39


OPERATOR NAME:
QUINTON L DINOVI
PERMIT NUMBER: 210224
EXPIRATION DATE: 10/05/2023

LOT #: AG208102
SUPPLIER: INTOXIMETERS
EXPIRATION: 03/22/2024
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.097

BLANK TEST	0.000	15:10
INTERNAL STANDARD	VERIFIED	15:10
EXTERNAL STANDARD	0.096	15:10
BLANK TEST	0.000	15:11

Average = 0.0960
Std Dev = 0.0000
Spread = 0.0000

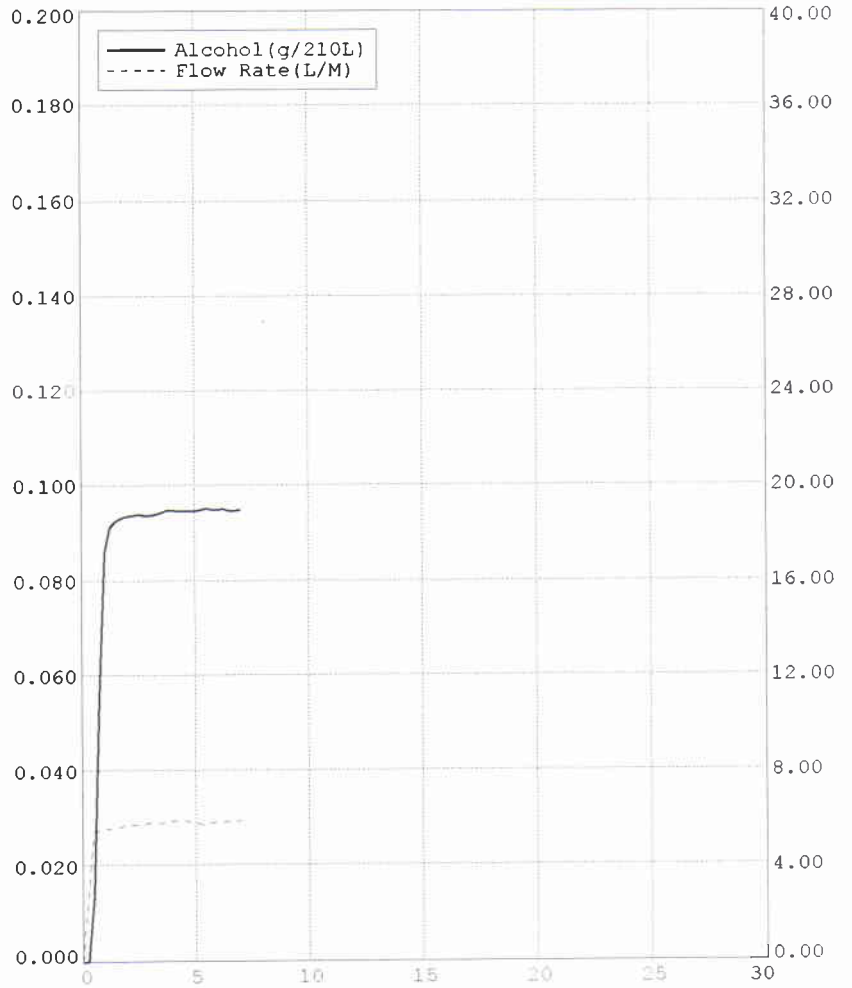



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
QUINTON L. DiNOVI

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 10/5/2021

Laura P. Way

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

NUMBER 210224

Donald A. Kamm

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

EXPIRES 10/5/2023

MO 580-0771 (6-10)

LAB-4 (R6-10)

 **STATE OF MISSOURI**
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator **DINOVI, QUINTON**
 Permit No **210224**
 Date Issued **10/5/2021** Date Expires **10/5/2023**

