

MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500027	NAME OF AGENCY Hillsboro Police Dept.	DATE OF INSPECTION 09/03/2023
LOCATION OF INSTRUMENT (STREET AND CITY) 101 Main Street 63050		TIME OF INSPECTION 13:29:14

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>09/03/2023 13:29:16</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.9°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>44.4°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD  COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG314401 EXP. DATE 05/24/2025

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_ SIM. SN \_\_\_\_\_ SIM. NIST EXP DATE \_\_\_\_\_

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)  
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.078	TEST 2: 0.077	TEST 3: 0.078
---------------	---------------	---------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 1	.10-.14: 2	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

standard change

**INSPECTING OFFICER**

SIGNATURE <i>Brian J Magnan</i>	PRINT FULL NAME BRIAN J MAGNAN
TYPE II PERMIT NUMBER 210312	EXPIRATION DATE 12/14/2023
	TELEPHONE NUMBER 636-300-2800

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email



**Airgas USA LLC (LAB)**  
 3500 Bernard Street  
 St. Louis, Mo. 63103  
 Ph: (314) 533-3100  
 Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**  
 Exclusive Supplier  
 Intoximeters, Inc.  
 2081 Craig Road  
 St. Louis, Mo 63146

**Test Date:** 24-May-2023

**Lot # AG314401    Model 108**

<b>Exp Date</b> 24-May-2025	<b>Cyl. Type</b> 108	<b>Component</b> Ethanol Nitrogen	<b>Certified Concentration</b> 0.080 ± 0.002 BrAC (208.4 ppm)
--------------------------------	-------------------------	---	--

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

**Analytical Method:** NDIR

Digitally signed by Quality Control  
 Reason: Dry gas standard certification of analysis  
 Location: Airgas USA LLC (Lab)  
 Date: 05.24.2023 17:28

**Approved for Release:** \_\_\_\_\_  
  
 Rod Marsala

**ISO 17025:2017 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**

STANDARD CHANGE

Hillsboro Police Dept.  
INTOX dmt: 500027

Date: 09/03/2023  
Time: 13:25:38


OPERATOR NAME:  
BRIAN J MAGNAN  
PERMIT NUMBER: 210312  
EXPIRATION DATE: 12/14/2023

LOT #: AG314401  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 05/24/2025  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.080  
TARGET: 0.078

BLANK TEST	0.000	13:26
INTERNAL STANDARD	VERIFIED	13:26
EXTERNAL STANDARD	0.076	13:26
BLANK TEST	0.000	13:27

Average = 0.0760  
Std Dev = 0.0000  
Spread = 0.0000

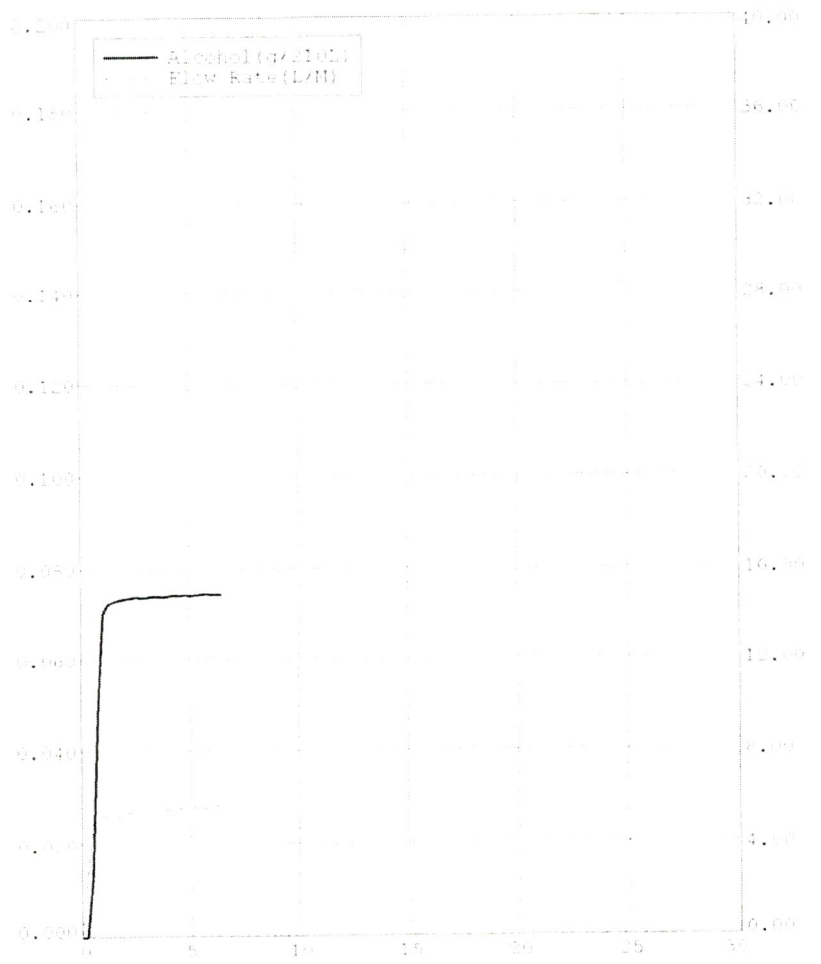

CPL B. Magnan #357





STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



**PERMIT**  
**TYPE II**  
**BRIAN J. MAGNAN**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 12/14/2021

NUMBER 210312

EXPIRES 12/14/2023

*Laura P. Day*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Donald A. Kamm*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

 **STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*

**Operator** MAGNAN, BRIAN  
**Permit No** 210312  
**Date Issued** 12/14/2021 **Date Expires** 12/14/2023

