



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

**RECEIVED**  
 By Tracy Crews at 8:03 am, Sep 11, 2023

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

|   |   |                                  |
|---|---|----------------------------------|
| INTOX DMT SN<br>500180  | NAME OF AGENCY<br>Missouri State Highway Patrol | DATE OF INSPECTION<br>09/09/2023 |
| LOCATION OF INSTRUMENT (STREET AND CITY)<br>1 Court Circle, Camdenton, Missouri 65020 |   | TIME OF INSPECTION<br>17:37:56   |

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

|  |   |
|--|---|
| DATE AND TIME <u>09/09/2023 17:38:00</u>                         | <input checked="" type="checkbox"/> DETECTOR          |
| <input checked="" type="checkbox"/> PROGRAM                      | <input checked="" type="checkbox"/> FILTER 1          |
| <input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u> | <input checked="" type="checkbox"/> FILTER 2          |
| <input checked="" type="checkbox"/> BREATH TUBE <u>46.2°C</u>    | <input checked="" type="checkbox"/> FILTER 3          |
| <input checked="" type="checkbox"/> PUMP                         | <input checked="" type="checkbox"/> INTERNAL STANDARD |

**BREATH ANALYZER ACCURACY STANDARDS**

SIMULATOR STANDARD       COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS      LOT # AG234103      EXP. DATE 12/07/2024

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_      SIM. SN \_\_\_\_\_      SIM. NIST EXP DATE \_\_\_\_\_

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.098      TEST 2: 0.098      TEST 3: 0.098

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

|             |          |            |            |            |             |
|-------------|----------|------------|------------|------------|-------------|
| REFUSALS: 0 | 0-.04: 0 | .05-.09: 0 | .10-.14: 0 | .15-.19: 0 | OVER .19: 0 |
|-------------|----------|------------|------------|------------|-------------|

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

CHANGED DRY GAS

**INSPECTING OFFICER**

|                             |                                 |
|-----------------------------|---------------------------------|
| SIGNATURE<br><i>T. Rosa</i> | PRINT FULL NAME<br>TYLER R ROSA |
|-----------------------------|---------------------------------|

|                                 |                               |                                  |
|---------------------------------|-------------------------------|----------------------------------|
| TYPE II PERMIT NUMBER<br>230121 | EXPIRATION DATE<br>06/07/2025 | TELEPHONE NUMBER<br>573-751-1000 |
|---------------------------------|-------------------------------|----------------------------------|

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services  
 by mail, fax, or email

STANDARD CHANGE

-----  
Missouri State Highway Patrol  
INTOX dmt: 500180  
-----

Date: 09/09/2023  
Time: 17:34:42

OPERATOR NAME:  
TYLER R ROSA  
PERMIT NUMBER: 230121  
EXPIRATION DATE: 06/07/2025


LOT #: AG234103  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 12/07/2024  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.097

|                   |          |       |
|-------------------|----------|-------|
| BLANK TEST        | 0.000    | 17:35 |
| INTERNAL STANDARD | VERIFIED | 17:35 |
| EXTERNAL STANDARD | 0.097    | 17:36 |
| BLANK TEST        | 0.000    | 17:36 |

Average = 0.0970  
Std Dev = 0.0000  
Spread = 0.0000

*T. Rosa*

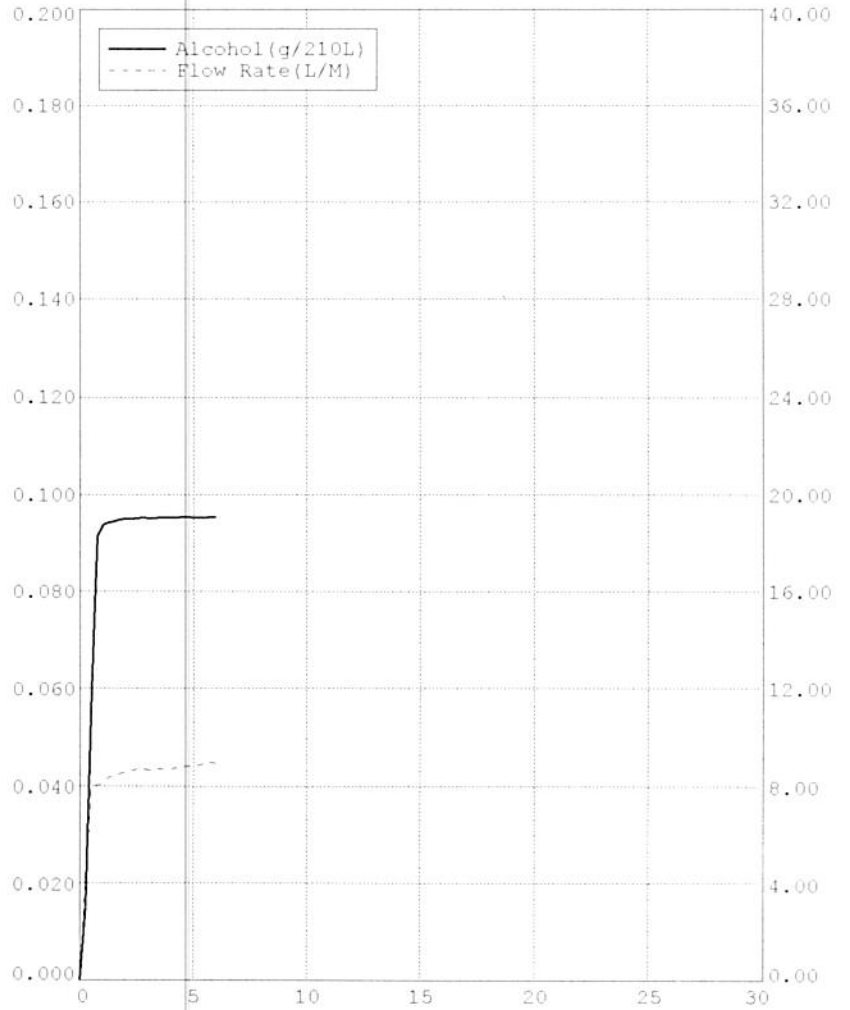



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



**PERMIT**  
**TYPE II**  
**TYLER ROSA**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**ALCO-SENSOR IV WITH PRINTER, INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 6/7/2023

NUMBER 230121

EXPIRES 6/7/2025

*Mike Massman*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*Paula J. Nicholson*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES



**STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*

**Operator** ROSA, TYLER  
**Permit No** 230121  
**Date Issued** 6/7/2023    **Date Expires** 6/7/2025

