



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

RECEIVED
 By Tracy Crews at 8:03 am, Sep 11, 2023

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500180	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 09/09/2023
LOCATION OF INSTRUMENT (STREET AND CITY) 1 Court Circle, Camdenton, Missouri 65020		TIME OF INSPECTION 17:26:16

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>09/09/2023 17:26:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.2°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG234103 EXP. DATE 07/12/2024

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: **0.098** TEST 2: **0.098** TEST 3: **0.101**

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 1	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Changed Dry Gas

INSPECTING OFFICER

SIGNATURE <i>T. Rosa</i>	PRINT FULL NAME TYLER R ROSA
-----------------------------	--

TYPE II PERMIT NUMBER 230121	EXPIRATION DATE 06/07/2025	TELEPHONE NUMBER 573-751-1000
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE
 Breath Alcohol Program, Missouri Department of Health and Senior Services
 by mail, fax, or email

STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500180

Date: 09/09/2023
Time: 17:22:53

OPERATOR NAME:
TYLER R ROSA
PERMIT NUMBER: 230121
EXPIRATION DATE: 06/07/2025


LOT #: AG234103
SUPPLIER: INTOXIMETERS
EXPIRATION: 07/12/2024
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.097

BLANK TEST	0.000	17:23
INTERNAL STANDARD	VERIFIED	17:23
EXTERNAL STANDARD	0.097	17:24
BLANK TEST	0.000	17:25

Average = 0.0970
Std Dev = 0.0000
Spread = 0.0000

T. Rosa

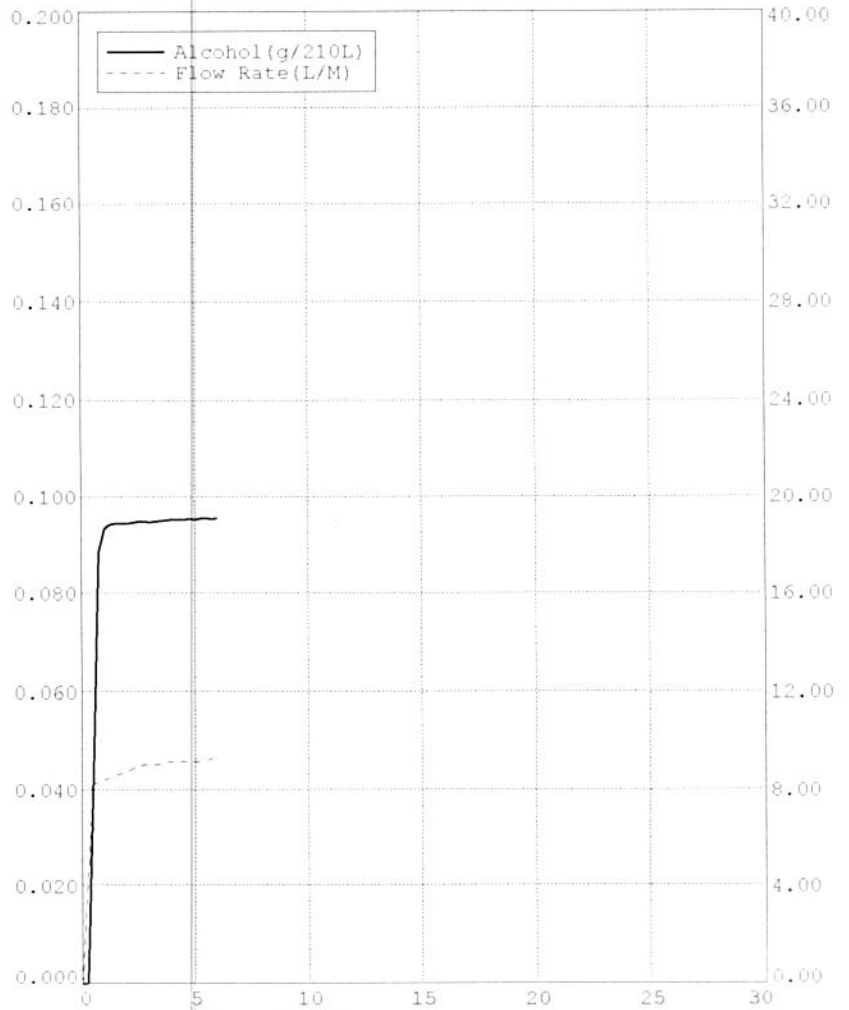



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
TYLER ROSA

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

ALCO-SENSOR IV WITH PRINTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 6/7/2023

NUMBER 230121

EXPIRES 6/7/2025

Mike Massman

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

Paula J. Nielson

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

 **STATE OF MISSOURI**
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator ROSA, TYLER
Permit No 230121
Date Issued 6/7/2023 **Date Expires** 6/7/2025

