



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

**INTOX DMT MAINTENANCE REPORT**

**RECEIVED**

By Tracy Crews at 2:07 pm, Sep 08, 2023

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500205	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 08/31/2023
LOCATION OF INSTRUMENT (STREET AND CITY) 2920 N. Shamrock Rd, Jefferson City		TIME OF INSPECTION 11:29:51

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>08/31/2023 11:29:53</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>45.5°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG320501</u>	EXP. DATE <u>07/24/2025</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____	SIM. NIST EXP DATE _____

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.098	TEST 2: 0.098	TEST 3: 0.098
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST
---

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Detector Replaced and Detector Block cleaned. Standard change performed and Instrument calibrated.

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME JIMMY L CLEVELAND	
TYPE II PERMIT NUMBER 230082	EXPIRATION DATE 05/03/2025	TELEPHONE NUMBER 573-751-4722

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email

CALIBRATION FACTORS

-----  
Missouri State Highway Patrol  
INTOX dmt: 500205  
-----

Date: 08/30/2023  
Time: 13:41:30

OPERATOR NAME:  
JIMMY L CLEVELAND  
PERMIT NUMBER: 230082  
EXPIRATION DATE: 05/03/2025  
MISC:  
MP2316

LOT #: 23180  
SUPPLIER: GUTH  
EXPIRATION: 05/17/2025

Ca = 0.1000  
ADJ = 0.980927    0.800 <= ADJ < 1.200  
b1 = 0.0000    0.0000 <= b1 < 0.0040  
b2 = 0.0018    0.0010 <= b2 < 0.0100  
b3 = 0.0000    0.0000 <= b3 < 0.0040  
Xq = 0.1144    0.0500 <= Xq < 0.2500  
a21 = 1.097556    1.050 <= a21 < 1.300  
a31 = 0.392438    0.300 <= a31 < 0.800

*Post Vn*

STANDARD CHANGE

Missouri State Highway Patrol  
INTOX dmt: 500205

Date: 08/30/2023  
Time: 12:57:41


OPERATOR NAME:  
JIMMY L CLEVELAND  
PERMIT NUMBER: 230082  
EXPIRATION DATE: 05/03/2025

LOT #: AG320501  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 07/24/2025  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.098

BLANK TEST	0.000	12:58
INTERNAL STANDARD	VERIFIED	12:58
EXTERNAL STANDARD	0.096	12:59
BLANK TEST	0.000	12:59

Average = 0.0960  
Std Dev = 0.0000  
Spread = 0.0000

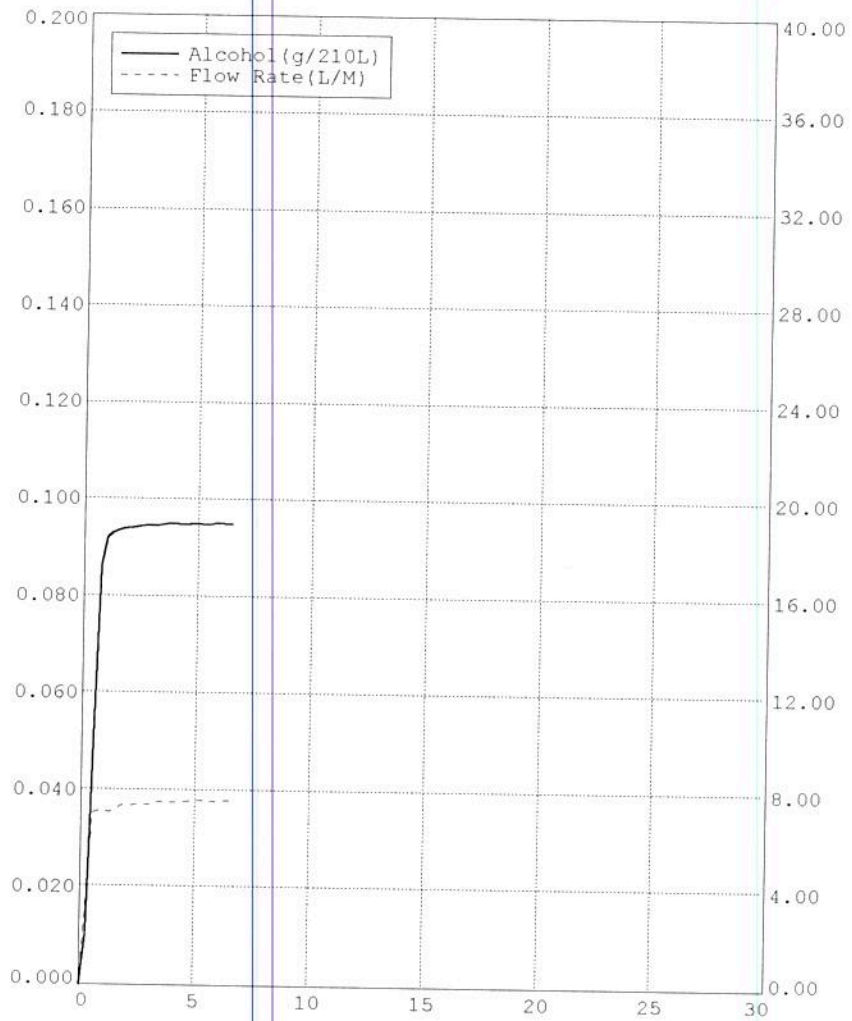

90806



Airgas USA LLC (LAB)  
3500 Bernard Street  
St. Louis, Mo. 63103  
Ph: (314) 533-3100  
Fax: (314) 533-7328

# Certificate of Analysis

**Customer Name**  
Exclusive Supplier  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 26-Jul-2023

**Lot #** AG320501 **Model** 108

<b>Exp Date</b> 24-Jul-2025	<b>Cyl. Type</b> 108	<b>Component</b> Ethanol Nitrogen	<b>Certified Concentration</b> 0.100 ± 2% BrAC (260 ppm)
--------------------------------	-------------------------	---	---

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010562	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

**Analytical Method:** NDIR

Digitally signed by:Quality Control  
Reason:Dry gas standard certification of analysis  
Location:Airgas USA LLC (Lab)  
Date:07.26.2023 12:45

Approved for Release:   
Rod Marsala

**ISO 17025:2017 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**





# GUTH LABORATORIES, INC.

590 NORTH 67th STREET • HARRISBURG, PA 17111-4511 • TELEPHONE: 717-564-5470

## CERTIFICATE OF ANALYSIS

Certified Alcohol Reference Solution for Simulator

Random Samples of Lot Number **23180** of Alcohol Reference Solution for Simulator were analyzed by gas chromatography on **May 18, 2023**, using a Perkin Elmer Gas Chromatograph Autosystem XL S/N: 610N9030209, and found to contain **0.1220%** (w/vol) ethyl alcohol. The expiration date for this lot number is **May 17, 2025** at 11:59 PM.

When used in a calibrated Simulator, operating at  $34^{\circ}\text{C} \pm .2^{\circ}\text{C}$ , this solution will give a breath alcohol analysis instrument reading of **0.100 g/210L  $\pm$  3%**.

The alcohol and water used in this solution were free of test interfering substances.

Ted L. Pauley, President  
GUTH LABORATORIES, INC.

*NIST Traceability:*

*Testing was conducted using Cerilliant Reference Standard lot number FN11172002 whose values are traceable to NIST.*

*All balances are calibrated annually by an outside agency using NIST traceable weights. Calibration verification is done prior to each use utilizing NIST traceable weights.*



STATE OF MISSOURI  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

2

**PERMIT  
TYPE II**

**JIMMY L. CLEVELAND**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repair and operate the following breath analyzer(s):

**ALCO-SENSOR IV WITH PRINTER, INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 5/3/2023

NUMBER 230082

EXPIRES 5/3/2025

*Mike Massman*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

*David J. Nicholson*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MD 580-0771 (E-10)

LAB-4 (REV)



**STATE OF MISSOURI**  
DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

**Operator** CLEVELAND, JIMMY  
**Permit No** 230082  
**Date Issued** 5/3/2023    **Date Expires** 5/3/2025

