



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

RECEIVED
 by 7/15/23 11:00 am, 8/1/23

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500258	NAME OF AGENCY Mountain Grove Police Department	DATE OF INSPECTION 09/15/2023
LOCATION OF INSTRUMENT (STREET AND CITY) Mountain Grove Police 102 East State Street		TIME OF INSPECTION 14:49:38

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>09/15/2023 14:49:40</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER GUTH LOT # 302402655996 EXP. DATE 02/08/2026

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.096 TEST 2: 0.098 TEST 3: 0.097

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0 0-.04: 0 .05-.09: 0 .10-.14: 0 .15-.19: 0 OVER .19: 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE *Danny Sprague* PRINT FULL NAME **DANNY SPRAGUE**

TYPE II PERMIT NUMBER **230173** EXPIRATION DATE **08/08/2025** TELEPHONE NUMBER _____

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, Missouri Department of Health and Senior Services**
 by mail, fax, or email

STANDARD CHANGE

Mountain Grove Police Department
INTOX dmt: 500258

Date: 09/15/2023
Time: 14:40:42


OPERATOR NAME:
DANNY SPRAGUE
PERMIT NUMBER: 230173
EXPIRATION DATE: 08/08/2025

LOT #: 302402655996
SUPPLIER: GUTH
EXPIRATION: 02/08/2026
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.095

BLANK TEST	0.000	14:41
INTERNAL STANDARD	VERIFIED	14:41
EXTERNAL STANDARD	0.094	14:42
BLANK TEST	0.000	14:42

Average = 0.0940
Std Dev = 0.0000
Spread = 0.0000

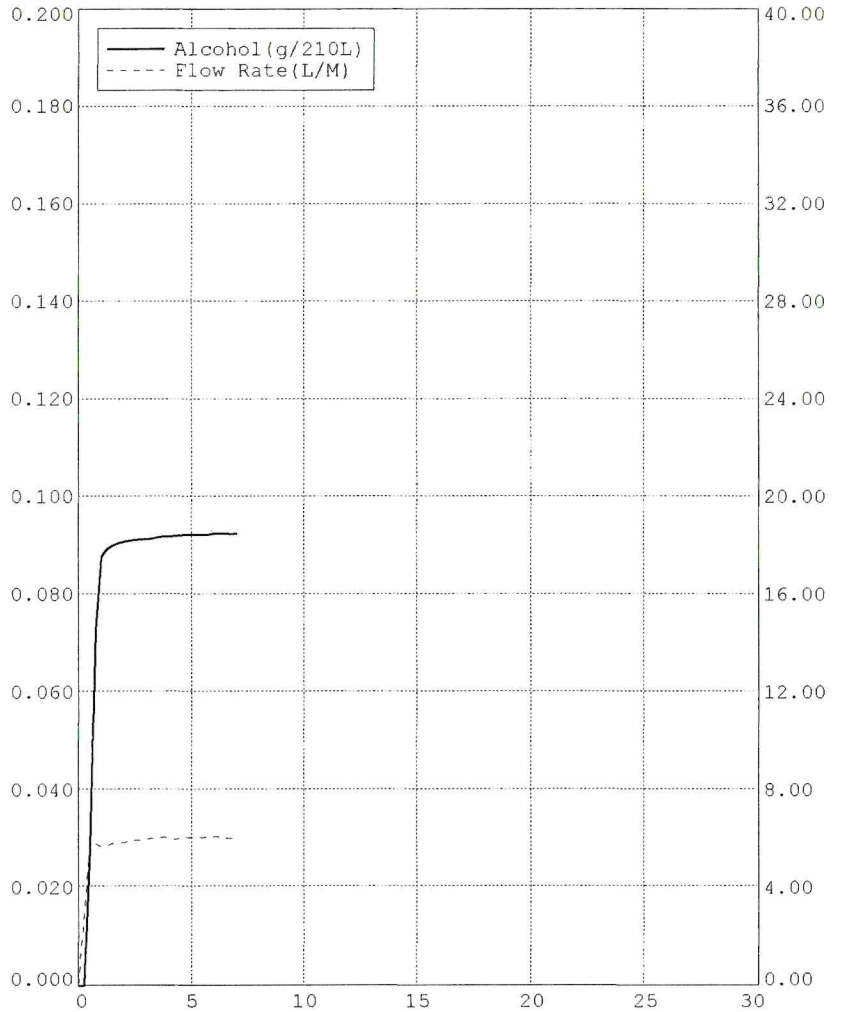

Danny Sprague