



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

RECEIVED

By Tracy Crews at 11:24 am, Nov 28, 2023

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500268	NAME OF AGENCY Pettis County Jail	DATE OF INSPECTION 11/27/2023
LOCATION OF INSTRUMENT (STREET AND CITY) 333 S Lamine Ave, Sedalia, Pettis County, MO		TIME OF INSPECTION 05:18:17

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>11/27/2023 05:18:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG220101 EXP. DATE 07/20/2024

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.078	TEST 2: 0.078	TEST 3: 0.078
---------------	---------------	---------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 5	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------


LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Instrument is operating within standards and guidelines established by MODHSS

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME DUSTIN R SOUTHARD	
TYPE II PERMIT NUMBER 210323	EXPIRATION DATE 12/16/2023	TELEPHONE NUMBER 660-827-0052

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901

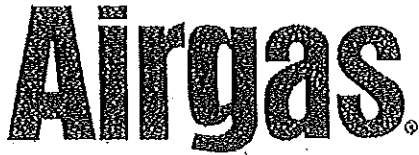

Airgas USA LLC (LAB)
 3500 Bernard Street
 St. Louis, Mo. 63103
 Ph: (314) 533-3100
 Fax: (314) 633-7328

Certificate of Analysis

Customer Name
 Exclusive Supplier
 Intoximeters, Inc.
 2081 Cralg Road
 St. Louis, Mo 63146

Test Date: 20-Jul-2022

Lot # AG220101 Model 108

Exp Date	Cyl. Type	Component	Certified Concentration
20-Jul-2024	108	Ethanol Nitrogen	0.080 ± 0.002 BrAC (208 ppm)

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.	Concentration	RGM Serial No.	Concentration
EB0010581	391.8 ppm	EB0010603	392.5 ppm
EB0010570	259.8 ppm	EB0010559	258.9 ppm
EB0010285	209.0 ppm	EB0010582	104.2 ppm
EB0010561	103.7 ppm	EB0010579	52.94 ppm
EB0010681	52.22 ppm		

CRM Serial No.	Concentration	CRM Serial No.	Concentration
CC727481	800.0 ppm	CC727493	390.0 ppm
CC727496	253.0 ppm	CC727498	150.0 ppm

Analytical Method: NDIR

Digitally signed by: Quality Control
 Reason: Dry gas standard certification of analysis
 Location: Airgas USA LLC (Lab)
 Date: 07.20.2022 18:37

Approved for Release: _____

Rod Marsala

ISO 17025:2017 A2LA accredited. Certificate Number 3082.06
 ISO 17034:2016 A2LA accredited. Certificate Number 3082.07



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

**PERMIT
 TYPE II**

DUSTIN R. SOUTHARD

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

ALCO-SENSOR IV WITH PRINTER, INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 12/16/2021

NUMBER 210323

EXPIRES 12/16/2023

Laura Q. Day

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

Donald A. Ramsey

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)

 **STATE OF MISSOURI**
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator SOUTHARD, DUSTIN
 Permit No 210323
 Date Issued 12/16/2021 Date Expires 12/16/2023

