



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM  
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500115	NAME OF AGENCY Missouri State Highway Patrol, Troop B - Zone 6	DATE OF INSPECTION 02/07/2024
LOCATION OF INSTRUMENT (STREET AND CITY) 117 S. Market St., Rm #3, Memphis, Scotland CO SO		TIME OF INSPECTION 15:45:40

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>02/07/2024 15:45:42</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.3°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD  COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG320502 EXP. DATE 07/24/2025

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_ SIM. SN \_\_\_\_\_ SIM. NIST EXP DATE \_\_\_\_\_

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)  
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.098	TEST 2: 0.097	TEST 3: 0.097
---------------	---------------	---------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 1	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

MEETS DHSS STANDARDS. ADJUSTED TIME.

INSPECTING OFFICER

SIGNATURE <i>Zachary S Horrell</i>	PRINT FULL NAME ZACHARY S HORRELL
TYPE II PERMIT NUMBER 240034	TELEPHONE NUMBER 660-385-2132
EXPIRATION DATE 02/05/2026	

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services by mail, fax, or email



**Airgas USA LLC (LAB)**  
 3500 Bernard Street  
 St. Louis, Mo. 63103  
 Ph: (314) 533-3100  
 Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**  
*Exclusive Supplier*  
 Intoximeters, Inc.  
 2081 Craig Road  
 St. Louis, Mo 63146

**Test Date:** 1-Aug-2023

**Lot #** AG320502 **Model** 108

Exp Date	Cyl. Type	Component	Certified Concentration
24-Jul-2025	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm)

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

RGM Serial No.	Concentration
EB0010581	391.8 ppm
EB0010570	259.8 ppm
EB0010285	209.0 ppm
EB0010561	103.7 ppm
EB0010681	52.22 ppm

RGM Serial No.	Concentration
EB0010603	392.5 ppm
EB0010559	258.9 ppm
EB0010562	104.2 ppm
EB0010579	52.94 ppm

CRM Serial No.	Concentration
CC727481	800.0 ppm
CC727496	253.0 ppm

CRM Serial No.	Concentration
CC727493	390.0 ppm
CC727498	150.0 ppm

**Analytical Method:** NDIR

Digitally signed by: Quality Control  
 Reason: Dry gas standard certification of analysis  
 Location: Airgas USA LLC (Lab)  
 Date: 08.10.2023 09:48

**Approved for Release:** \_\_\_\_\_  
 Yusef Woods

**ISO 17025:2017 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**

STANDARD CHANGE

Missouri State Highway Patrol, Troop B -  
Zone 6  
INTOX dmt: 500115

Date: 02/07/2024  
Time: 15:42:01


OPERATOR NAME:  
ZACHARY S HORRELL  
PERMIT NUMBER: 240034  
EXPIRATION DATE: 02/05/2026

LOT #: AG320502  
SUPPLIER: INTOXIMETERS  
EXPIRATION: 07/24/2025  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.097

BLANK TEST	0.000	15:42
INTERNAL STANDARD	VERIFIED	15:43
EXTERNAL STANDARD	0.095	15:43
BLANK TEST	0.000	15:44

Average = 0.0950  
Std Dev = 0.0000  
Spread = 0.0000

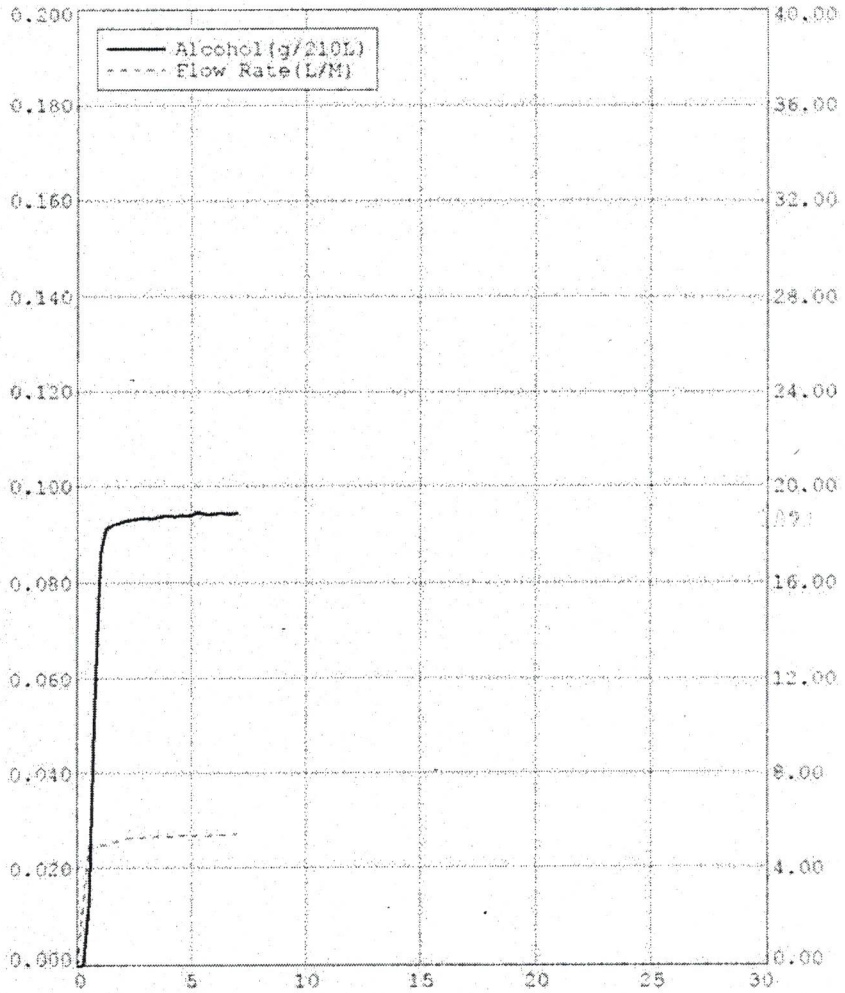

*Tpr. Z. Horrell*



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

2

**PERMIT**  
**TYPE II**  
**ZACHARY S. HORRELL**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 2/5/2024

*Mike Masman*

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

NUMBER 240034

*Paula J. Nickelson*

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

EXPIRES 2/5/2026

 STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*

Operator HORRELL, ZACHARY  
 Permit No 240034  
 Date Issued 2/5/2024 Date Expires 2/5/2026

