

RECEIVED

By Tracy Crews at 8:47 am, Jan 18, 2024



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500217	NAME OF AGENCY KIMBERLING CITY PD	DATE OF INSPECTION 01/17/2024
------------------------	--------------------------------------	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 34 KIMBERLING BLVD KIMBERLING CITY, MO 65686	TIME OF INSPECTION 11:04:38
--	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>01/17/2024 11:04:40</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>45.5°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG334602</u>	EXP. DATE <u>12/12/2025</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____	SIM. NIST EXP DATE _____
--	---------------	--------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.102	TEST 2: 0.101	TEST 3: 0.102
---------------	---------------	---------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

New Gas - Monthly Main

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME TODD N LEMOINE
---------------	-----------------------------------

TYPE II PERMIT NUMBER 220223	EXPIRATION DATE 09/09/2024	TELEPHONE NUMBER 417-739-2131
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services
by mail, fax, or email

STANDARD CHANGE

KIMBERLING CITY PD
INTOX dmt: 500217

Date: 01/17/2024
Time: 11:14:48


OPERATOR NAME:
TODD N LEMOINE
PERMIT NUMBER: 220223
EXPIRATION DATE: 09/09/2024
MISC:
NEW GAS

LOT #: AG334602
SUPPLIER: INTOXIMETERS
EXPIRATION: 12/12/2025
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.097

BLANK TEST	0.000	11:15
INTERNAL STANDARD	VERIFIED	11:15
EXTERNAL STANDARD	0.099	11:16
BLANK TEST	0.000	11:17

Average = 0.0990
Std Dev = 0.0000
Spread = 0.0000

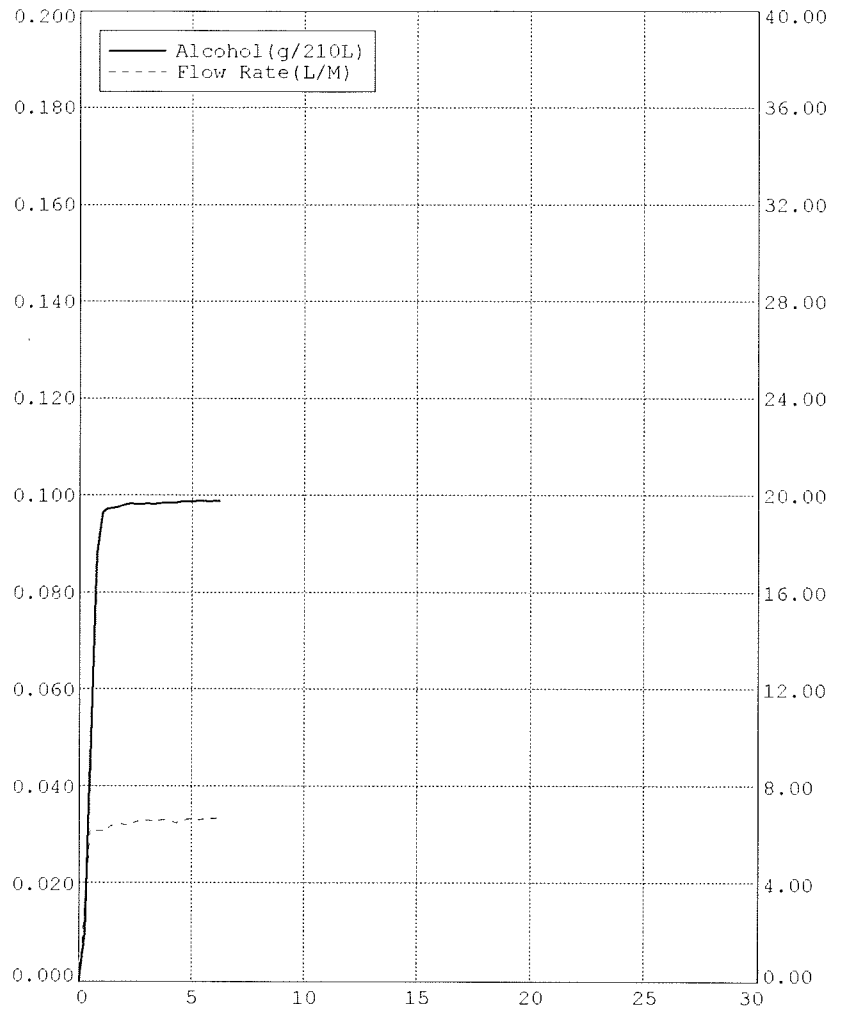

Todd N Lemoine