



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

**INTOX DMT MAINTENANCE REPORT**

**RECEIVED**

By Tracy Crews at 4:08 pm, Apr 10, 2020

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN <b>500222</b>	NAME OF AGENCY <b>Cape Girardeau Police Department</b>	DATE OF INSPECTION <b>04/08/2020</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO</b>		TIME OF INSPECTION <b>21:44:15</b>

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>04/08/2020 21:44:17</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.8°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
---	--

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG916303</u>	EXP. DATE <u>06/12/2021</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.081	TEST 2: 0.080	TEST 3: 0.080
---------------	---------------	---------------

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Maintenance

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME <b>JACOB W MARBERRY</b>
---------------	--

TYPE II PERMIT NUMBER <b>280323</b>	EXPIRATION DATE <b>11/19/2020</b>	TELEPHONE NUMBER <b>573-335-6621</b>
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
Southeast District Office  
2875 James Blvd, Poplar Bluff, MO 63901



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**

*Exclusive Supplier*

Intoximeters, Inc.

2081 Craig Road

St. Louis, Mo 63146

**Test Date:** 15-Jun-2019

**Lot #** AG916303 **Model** 108cacd

**Exp. Date**

12-Jun-2021

**Cyl. Type**

108

**Component**

Ethanol

Nitrogen

**Certified Concentration**

0.080 ± 0.002 BrAC (208 ppm)

Balance

**Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:**

**RGM Serial No.**

EB0010581

EB0010570

EB0010285

EB0010561

EB0010681

**Concentration**

392.1 ppm

259.8 ppm

208.0 ppm

103.6 ppm

52.12 ppm

**RGM Serial No.**

EB0010603

EB0010559

EB0010595

EB0010562

EB0010579

**Concentration**

393.0 ppm

258.2 ppm

208.3 ppm

104.2 ppm

52.81 ppm

**CRM Serial No.**

CC434668

CC234503

**Concentration**

800.0 ppm

253.0 ppm

**CRM Serial No.**

0056649

0056662

**Concentration**

390.1 ppm

150.2 ppm

**Analytical Method:**

NDIR

Digitally signed by Quality Control  
Date: 2019.06.24 09:41:55 -05:00  
Reason: Dry gas standard certification of analysis  
Location: Airgas USA LLC (Lab)

Approved for Release:

Rod Marsala

**ISO 17025:2005 A2LA accredited. Certificate Number 3082.06**

**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



**PERMIT**  
**TYPE II**  
**JACOB W MARBERRY**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE **11/19/2018**

NUMBER **280323**

EXPIRES **11/19/2020**

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

**STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

*The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.*

**Operator** MARBERRY, JACOB  
**Permit No** 280323  
**Date Issued** 11/19/2018    **Date Expires** 11/19/2020

RECEIVED

By Tracy Crews at 9:54 am, Nov 19, 2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

APPROVED

By Stephen Wilson at 11:19 am, Nov 19, 2018

APPLICATION FOR TYPE II PERMIT FOR OPERATION OF BREATH ALCOHOL ANALYZERS

THIS APPLICATION IS FOR <input type="checkbox"/> NEW PERMIT <input checked="" type="checkbox"/> RENEWAL		CURRENT PERMIT NUMBER AND EXPIRATION DATE 260341 11-17-2018	
PRINT FULL NAME Jacob W Marberry		TITLE Patrolman	AGE 30
[REDACTED]		A disclosure concerning your SSN number is available at: <a href="http://www.health.mo.gov/lab/breathalcohol/">http://www.health.mo.gov/lab/breathalcohol/</a>	
DEPARTMENT OR TROOP Cape Girardeau MO Police		TELEPHONE (573) 335-6621	
BUSINESS ADDRESS (STREET, CITY, STATE, ZIP CODE) 2530 Maria Louise, Cape Girardeau, MO 63701			
EMAIL ADDRESS jmarberry@cityofcapegirardeau.org			

LIST ALL ORIGINAL TRAINING COURSES FOR OPERATION OF BREATH ANALYZERS  
(Also, please place a checkmark beside ALL breath analyzer(s) for which you are requesting a permit.)

DATES OF COURSE	LOCATION OF COURSE	COURSE LENGTH (HRS.)	NAME & MODEL OF BREATH ANALYZER	PLACE A / BESIDE INSTRUMENTS FOR WHICH YOU REQUEST	NAME OF INSTRUCTOR
2010	SEMO LE Academy	40	Datamaster	<input type="checkbox"/>	Eudy
10-2014	UCM/MSC	40	Type II Supervisor (IntoxDMT)	<input checked="" type="checkbox"/>	Welsh
11-2014	UCM/MSC	14	IntoxDMT	<input checked="" type="checkbox"/>	Welsh
				<input type="checkbox"/>	

List the manufacturer and name of instruments for which you are currently performing maintenance reports on and the number of maintenance reports performed on EACH type in the last year.

MANUFACTURER AND NAME OF INSTRUMENT	NUMBER OF MAINTENANCE REPORTS	NUMBER OF SUBJECT TESTS
1. IntoxDMT	2 <b>OK SGW</b>	5 Self Tests <b>OK SGW</b>
2.		
3.		

When adding a new instrument, you receive a new two (2) year permit. Therefore, normal renewal procedures apply for the instrument(s) on your current permit that you wish to transfer to the new permit. Disregarding these renewal procedures will result in a new permit for the new instrument only.

To renew a Type II Permit, the applicant shall have completed two (2) Maintenance Reports and shall have performed at least ten (10) tests on drinking subjects in the past year on each instrument for which renewal is requested. If these conditions are not met, or the permit has expired for more than thirty (30) days, the applicant shall perform two (2) Maintenance Reports and five (5) self-administered tests for each breath analyzer for which renewal is requested. Copies of the Maintenance Reports along with the Operational checklists and printouts for the five (5) self-administered tests shall accompany the application for renewal.

SIGNATURE OF APPLICANT 	DATE 11/18/2018
----------------------------	--------------------

RETURN COMPLETED APPLICATION TO THE: Breath Alcohol Program, Missouri Department of Health and Senior Services  
Southeast District Office  
2875 James Blvd.  
Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		INSTRUMENT SERIAL NUMBER 500222	DATE OF TEST 11/17/2018	TIME OF TEST 04:56:10
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	04:57
INTERNAL STANDARD	VERIFIED	04:57
SUBJECT SAMPLE (Vol=1.93L)	0.000	04:59
BLANK TEST	0.000	05:00

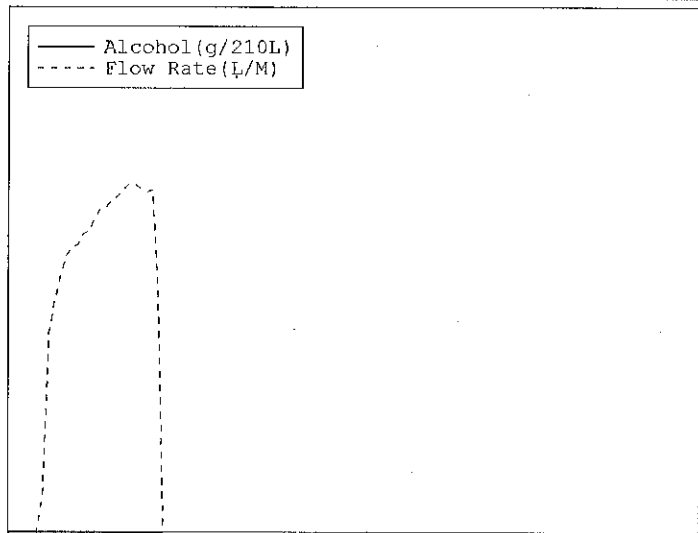

COMMENTS

CERTIFICATION BY OPERATOR

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

*J. Marberry*

DATE  
11/17/2018

WITNESS (IF ANY)

DATE  
11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN <b>500222</b>	NAME OF AGENCY <b>Cape Girardeau Police Department</b>	DATE OF INSPECTION <b>10/20/2018</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO</b>		TIME OF INSPECTION <b>08:52:17</b>

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>10/20/2018 08:52:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

SIMULATOR STANDARD       COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS      LOT # AG722402      EXP. DATE 08/12/2019

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_      SIMULATOR SN \_\_\_\_\_      SIMULATOR EXP DATE \_\_\_\_\_

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.079      TEST 2: 0.078      TEST 3: 0.078

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 1      0-.04: 13      .05-.09: 3      .10-.14: 2      .15-.19: 5      OVER .19: 2

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---



---

**INSPECTING OFFICER**

SIGNATURE       PRINT FULL NAME  
**JACOB W MARBERRY**

TYPE II PERMIT NUMBER 260341      EXPIRATION DATE 11/17/2018      TELEPHONE NUMBER 573-335-6621

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901**



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		INSTRUMENT SERIAL NUMBER 500222	DATE OF TEST 11/17/2018	TIME OF TEST 05:02:14
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	05:03
INTERNAL STANDARD	VERIFIED	05:03
SUBJECT SAMPLE (Vol=1.68L)	0.000	05:03
BLANK TEST	0.000	05:04

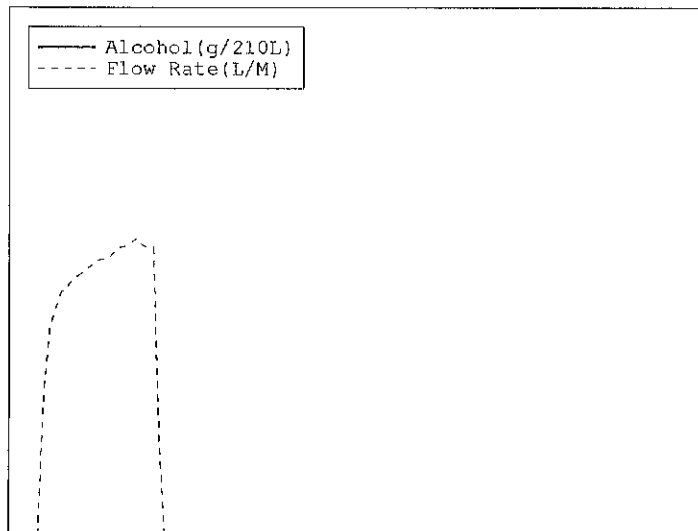

COMMENTS

CERTIFICATION BY OPERATOR

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

*J. Marberry*

DATE  
11/17/2018

WITNESS (IF ANY)

DATE  
11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500222	NAME OF AGENCY Cape Girardeau Police Department	DATE OF INSPECTION 10/20/2018
------------------------	--	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO	TIME OF INSPECTION 08:52:17
---	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>10/20/2018 08:52:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
---	--

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG722402</u>	EXP. DATE <u>08/12/2019</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
--	--------------------	--------------------------

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.079	TEST 2: 0.078	TEST 3: 0.078
---------------	---------------	---------------

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 1	0-.04: 13	.05-.09: 3	.10-.14: 2	.15-.19: 5	OVER .19: 2
-------------	-----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY
---------------	-------------------------------------

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901





MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		INSTRUMENT SERIAL NUMBER 500222	DATE OF TEST 11/17/2018	TIME OF TEST 05:06:15
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	05:07
INTERNAL STANDARD	VERIFIED	05:07
SUBJECT SAMPLE (Vol=1.81L)	0.000	05:08
BLANK TEST	0.000	05:09

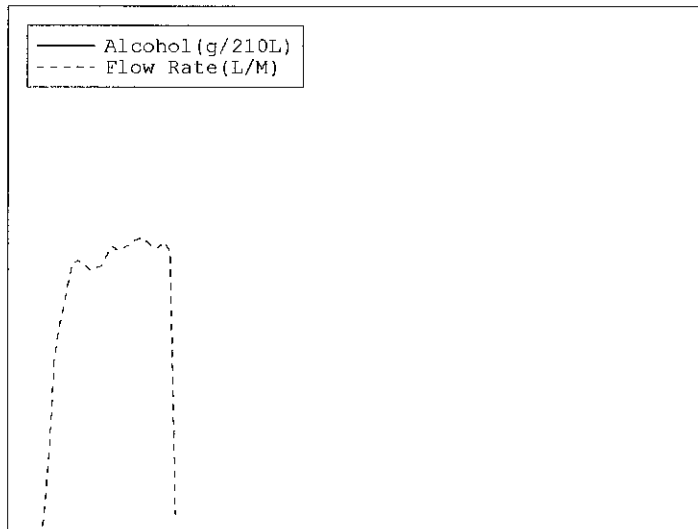

COMMENTS

CERTIFICATION BY OPERATOR

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

*Jacob Marberry*

DATE  
11/17/2018

WITNESS (IF ANY)

DATE  
11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500222	NAME OF AGENCY Cape Girardeau Police Department	DATE OF INSPECTION 10/20/2018
------------------------	--	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO	TIME OF INSPECTION 08:52:17
---	--------------------------------

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>10/20/2018 08:52:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG722402</u>	EXP. DATE <u>08/12/2019</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
--	--------------------	--------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: <u>0.079</u>	TEST 2: <u>0.078</u>	TEST 3: <u>0.078</u>
----------------------	----------------------	----------------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST
---

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 1	0-.04: 13	.05-.09: 3	.10-.14: 2	.15-.19: 5	OVER .19: 2
-------------	-----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY
---------------	-------------------------------------

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
**BLOOD ALCOHOL TEST REPORT - INTOX DMT**

FORM #11

LOCATION OF INSTRUMENT 2530 Maria Louise Ln.		INSTRUMENT SERIAL NUMBER 500223	DATE OF TEST 11/17/2018	TIME OF TEST 04:58:38
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

**OPERATIONAL CHECKLIST: INTOX DMT**

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

**SUBJECT TEST RESULTS**

BLANK TEST	0.000	04:59
INTERNAL STANDARD	VERIFIED	04:59
SUBJECT SAMPLE (Vol=1.79L)	0.000	05:00
BLANK TEST	0.000	05:01

— Alcohol (g/210L)  
 - - - - - Flow Rate (L/M)

COMMENTS

**CERTIFICATION BY OPERATOR**

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

BAC: 0.000

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR 	DATE 11/17/2018
WITNESS (IF ANY)	DATE 11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM

**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN <b>500223</b>	NAME OF AGENCY <b>Cape Girardeau PD</b>	DATE OF INSPECTION <b>10/20/2018</b>
LOCATION OF INSTRUMENT (STREET AND CITY) <b>2530 Maria Louise Ln.</b>		TIME OF INSPECTION <b>04:30:00</b>

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>10/20/2018 04:30:02</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
---	--

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG805701</u>	EXP. DATE <u>02/26/2020</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: <u>0.076</u>	TEST 2: <u>0.077</u>	TEST 3: <u>0.076</u>
----------------------	----------------------	----------------------

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: <u>2</u>	<u>0</u> - <u>04</u> : <u>98</u>	<u>05</u> - <u>09</u> : <u>0</u>	<u>10</u> - <u>14</u> : <u>0</u>	<u>15</u> - <u>19</u> : <u>0</u>	OVER <u>19</u> : <u>0</u>
--------------------	----------------------------------	----------------------------------	----------------------------------	----------------------------------	---------------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE 	PRINT FULL NAME <b>JACOB W MARBERRY</b>
--	--

TYPE II PERMIT NUMBER <b>260341</b>	EXPIRATION DATE <b>11/17/2018</b>	TELEPHONE NUMBER <b>573-335-6621</b>
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
Southeast District Office  
2875 James Blvd, Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
**BLOOD ALCOHOL TEST REPORT - INTOX DMT**

FORM #11


LOCATION OF INSTRUMENT 2530 Maria Louise Ln.		INSTRUMENT SERIAL NUMBER 500223	DATE OF TEST 11/17/2018	TIME OF TEST 05:03:29
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

**OPERATIONAL CHECKLIST: INTOX DMT**

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

**SUBJECT TEST RESULTS**

BLANK TEST	0.000	05:04
INTERNAL STANDARD	VERIFIED	05:04
SUBJECT SAMPLE (Vol=1.69L)	0.000	05:04
BLANK TEST	0.000	05:05

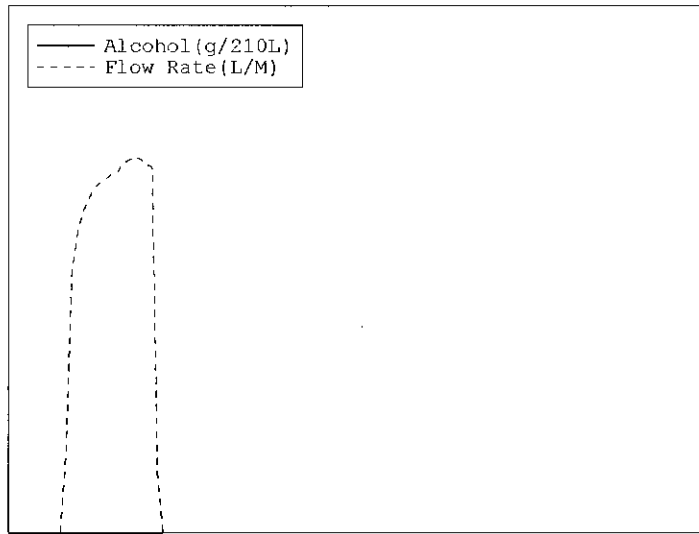

COMMENTS

**CERTIFICATION BY OPERATOR**

BAC  
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR <i>Jacob W Marberry</i>	DATE 11/17/2018
WITNESS (IF ANY)	DATE 11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500223	NAME OF AGENCY Cape Girardeau PD	DATE OF INSPECTION 10/20/2018
LOCATION OF INSTRUMENT (STREET AND CITY) 2530 Maria Louise Ln.		TIME OF INSPECTION 04:30:00

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

**DIAGNOSTIC RECORD**

DATE AND TIME <u>10/20/2018 04:30:02</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

**BREATH ANALYZER ACCURACY STANDARDS**

SIMULATOR STANDARD       COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS      LOT # AG805701      EXP. DATE 02/26/2020

SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_      SIMULATOR SN \_\_\_\_\_      SIMULATOR EXP DATE \_\_\_\_\_

**CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)**  
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.076      TEST 2: 0.077      TEST 3: 0.076

**PERFORM R.F.I. TEST**

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 2	0-.04: 98	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 0
-------------	-----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

---



---



---



---

**INSPECTING OFFICER**

SIGNATURE <i>JW 345</i>	PRINT FULL NAME JACOB W MARBERRY
----------------------------	-------------------------------------

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
 Southeast District Office  
 2875 James Blvd, Poplar Bluff, MO 63901



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**

Exclusive Supplier  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 14-Aug-2017

**Lot #** AG722402 **Model** 108cacd

**Exp. Date**

12-Aug-2019

**Cyl. Type**

108

**Component**

Ethanol  
Nitrogen

**Certified Concentration**

0.080 ± 0.002 BrAC (208 ppm)  
Balance

**Certification Traceable to N.I.S.T. RGM Ethanol Standards:**

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

**Analytical Method:**

NDIR

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**

Exclusive Supplier  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 26-Feb-2018

**Lot #** AG805701 **Model** 108cacd

**Exp. Date**

26-Feb-2020

**Cyl. Type**

108

**Component**

Ethanol  
Nitrogen

**Certified Concentration**

0.080 ± 0.002 BrAC (208 ppm)  
Balance

**Certification Traceable to N.I.S.T. RGM Ethanol Standards:**

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

**Analytical Method:**

NDIR

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01