



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500079	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 10/04/2020
-------------------------------	--	---

LOCATION OF INSTRUMENT (STREET AND CITY) 65 Business Park Dr., Troy, Missouri 63379	TIME OF INSPECTION 08:36:55
---	---------------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>10/04/2020 08:36:58</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>45.4°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG905201</u>	EXP. DATE <u>02/21/2021</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____	SIM. NIST EXP DATE _____

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.
<input checked="" type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.096	TEST 2: 0.096	TEST 3: 0.095
----------------------	----------------------	----------------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:					
REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 1	OVER .19: 1

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER	
SIGNATURE <i>Bryan W Long #855</i>	PRINT FULL NAME BRYAN W LONG
TYPE II PERMIT NUMBER 200038	TELEPHONE NUMBER 636-300-2800
EXPIRATION DATE 01/07/2022	

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, Missouri Department of Health and Senior Services
by mail, fax, or email



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 65 Business Park Dr., Troy, Missouri 63379	INSTRUMENT SERIAL NUMBER 500079	DATE OF TEST 10/22/2020	TIME OBSERVATION PERIOD STARTED 15:38	TIME OF TEST 15:53:01
SUBJECT NAME ALISSA D BEASLEY			DATE OF BIRTH 07/11/1975	
SUBJECT DRIVER'S LICENSE NUMBER X054230001			STATE MO	
ARRESTING OFFICER OFFICER A BEAN		ARRESTING OFFICER ID 2510		
OPERATOR SGT T CROFT		OPERATOR PERMIT 300058	PERMIT EXP DATE 01/03/2022	
OBSERVER SGT T CROFT		OBSERVER PERMIT 300058	PERMIT EXP DATE 01/03/2022	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by SGT T CROFT. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	15:53
INTERNAL STANDARD	VERIFIED	15:54
SUBJECT SAMPLE (Vol=4.39L)	0.092	15:54
BLANK TEST	0.000	15:55

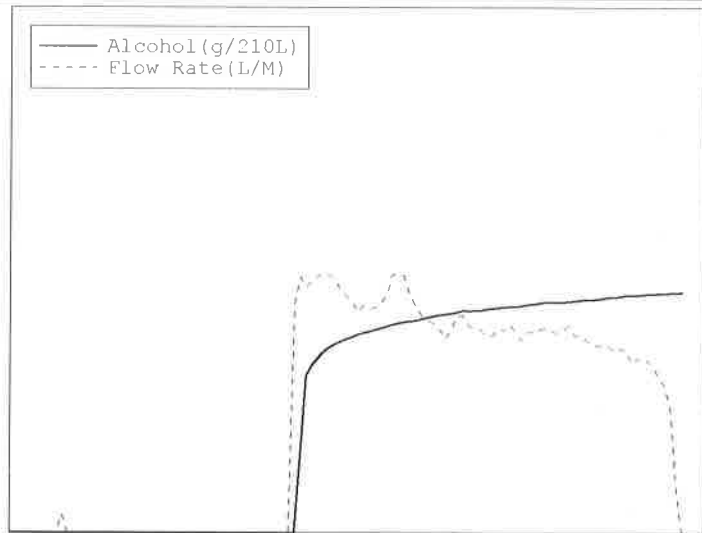

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.092

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.

SIGNATURE OF OPERATOR <i>T. Croft</i>	DATE 10/22/2020
WITNESS (IF ANY) <i>A. Bean</i>	DATE 10/22/2020



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 21-Feb-2019

Lot # AG905201 Model 108cacd

<u>Exp. Date</u> 21-Feb-2021	<u>Cyl. Type</u> 108	<u>Component</u> Ethanol Nitrogen	<u>Certified Concentration</u> 0.100 ± 2% BrAC (260 ppm) Balance
--	--------------------------------	--	---

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u> EB0010581 EB0010570 EB0010285 EB0010561 EB0010681	<u>Concentration</u> 392.1 ppm 259.8 ppm 208.0 ppm 103.6 ppm 52.12 ppm	<u>RGM Serial No.</u> EB0010603 EB0010559 EB0010595 EB0010562 EB0010579	<u>Concentration</u> 393.0 ppm 258.2 ppm 208.3 ppm 104.2 ppm 52.81 ppm
<u>CRM Serial No.</u> CC434668 CC234503	<u>Concentration</u> 800.0 ppm 253.0 ppm	<u>CRM Serial No.</u> 0056649 0056662	<u>Concentration</u> 390.1 ppm 150.2 ppm

Analytical Method: NDIR

Digitally signed by Quality Control
Date: 2019.02.21 15:31:31 -06:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06
ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

1573