

RECEIVED

By Tracy Crews at 8:51 am, Jun 11, 2020



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500098	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 06/02/2020
LOCATION OF INSTRUMENT (STREET AND CITY) Macon County SO, 101 E. Washington St., Macon, MO		TIME OF INSPECTION 18:30:40

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined) Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>06/02/2020 18:30:42</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>44.9°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG004403 EXP. DATE 02/13/2022

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.100 TEST 2: 0.099 TEST 3: 0.099

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS 0	0-.04: 0	.05-.09: 2	.10-.14: 1	.15-.19: 0	OVER .19: 0
------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME CHAD D PRIMM
---------------	---------------------------------

TYPE II PERMIT NUMBER 200094	EXPIRATION DATE 02/13/2022 - 2/18/22	TELEPHONE NUMBER 660-385-2132
---------------------------------	---	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
CHAD D PRIMM

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 2/18/2020

NUMBER 200094

EXPIRES 2/18/2022

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

MO 580-0771 (6-10)

LAB-4 (R6-10)



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator PRIMM, CHAD
Permit No 200094
Date Issued 2/18/2020 **Date Expires** 2/18/2022



STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500098

Date: 06/02/2020
Time: 18:23:21


OPERATOR NAME:
CHAD D PRIMM
PERMIT NUMBER: 200094
EXPIRATION DATE: 02/18/2022

LOT #: AG004403
SUPPLIER: INTOXIMETERS
EXPIRATION: 02/13/2022
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.096

BLANK TEST	0.000	18:24
INTERNAL STANDARD	VERIFIED	18:24
EXTERNAL STANDARD	0.096	18:24
BLANK TEST	0.000	18:25

Average = 0.0960
Std Dev = 0.0000
Spread = 0.0000

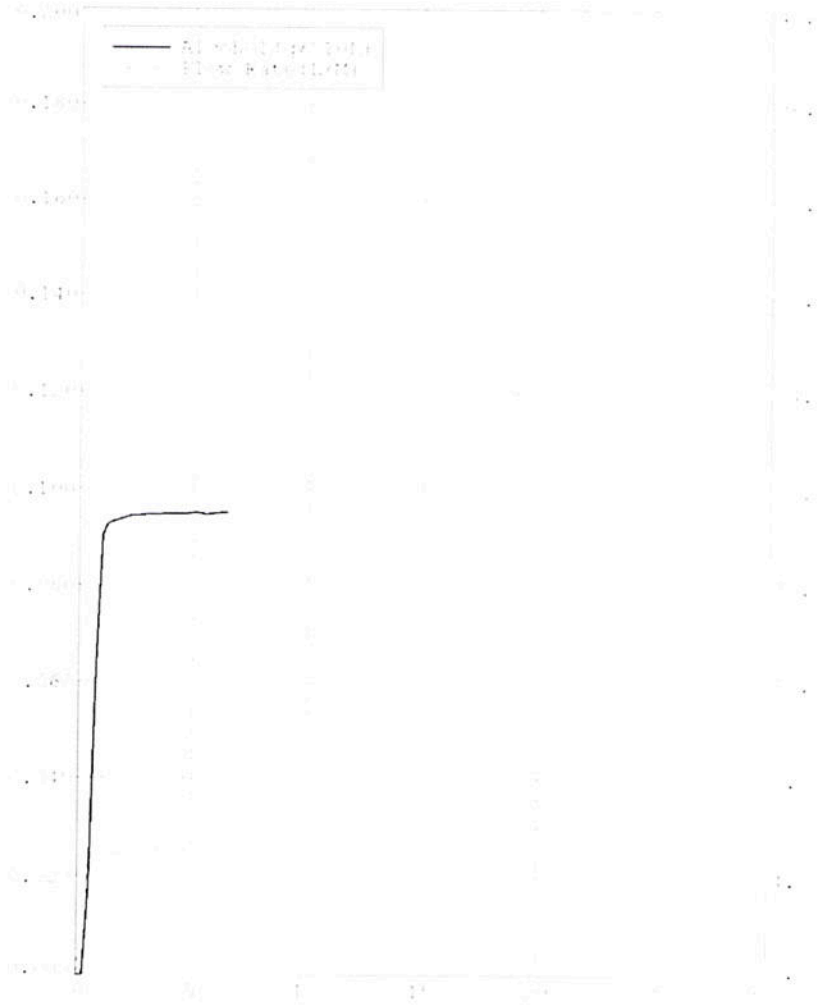

CDP #792