



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

RECEIVED
 07/16/2020 09:41:10 AM

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500137	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 06/06/2020
LOCATION OF INSTRUMENT (STREET AND CITY) 5 Basler Drive, Ste, Genevieve 63670		TIME OF INSPECTION 13:30:39

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>06/06/2020 13:30:41</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.3°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETER LOT # AG905201 EXP. DATE 02/21/2021

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.101 TEST 2: 0.101 TEST 3: 0.100

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 1	.10-.14: 0	.15-.19: 2	OVER .19: 4
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Fixed time and performed a standard change

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME DYLON M WYATT
TYPE II PERMIT NUMBER 200122	EXPIRATION DATE 03/03/2022
	TELEPHONE NUMBER 636-300-2800

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901**



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 21-Feb-2019

Lot # AG905201 Model 108cadd

Exp. Date

21-Feb-2021

Cyl. Type

108

Component

Ethanol
Nitrogen

Certified Concentration

0.100 ± 2% BrAC (260 ppm)
Balance

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

RGM Serial No.

EB0010581

EB0010570

EB0010285

EB0010561

EB0010681

Concentration

392.1 ppm

259.8 ppm

208.0 ppm

103.6 ppm

52.12 ppm

RGM Serial No.

EB0010603

EB0010559

EB0010595

EB0010562

EB0010579

Concentration

393.0 ppm

258.2 ppm

208.3 ppm

104.2 ppm

52.81 ppm

CRM Serial No.

CC434668

CC234503

Concentration

800.0 ppm

253.0 ppm

CRM Serial No.

0056649

0056662

Concentration

390.1 ppm

150.2 ppm

Analytical Method:

NDIR

Digitally signed by Quality Control
Date: 2019.02.21 15:31:31 -06:00
Reason: Dry gas standard certification of analysis
Location: Airgas USA LLC (Lab)

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06

ISO 17034:2016 A2LA accredited. Certificate Number 3082.07

STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500137

Date: 06/06/2020
Time: 13:26:53

OPERATOR NAME:
DYLAN M WYATT
PERMIT NUMBER: 200122
EXPIRATION DATE: 03/03/2022


LOT #: AG905201
SUPPLIER: INTOXIMETER
EXPIRATION: 02/21/2021
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.098

BLANK TEST	0.000	13:27
INTERNAL STANDARD	VERIFIED	13:27
EXTERNAL STANDARD	0.100	13:28
BLANK TEST	0.000	13:29

Average = 0.1000
Std Dev = 0.0000
Spread = 0.0000

DJ [Signature]

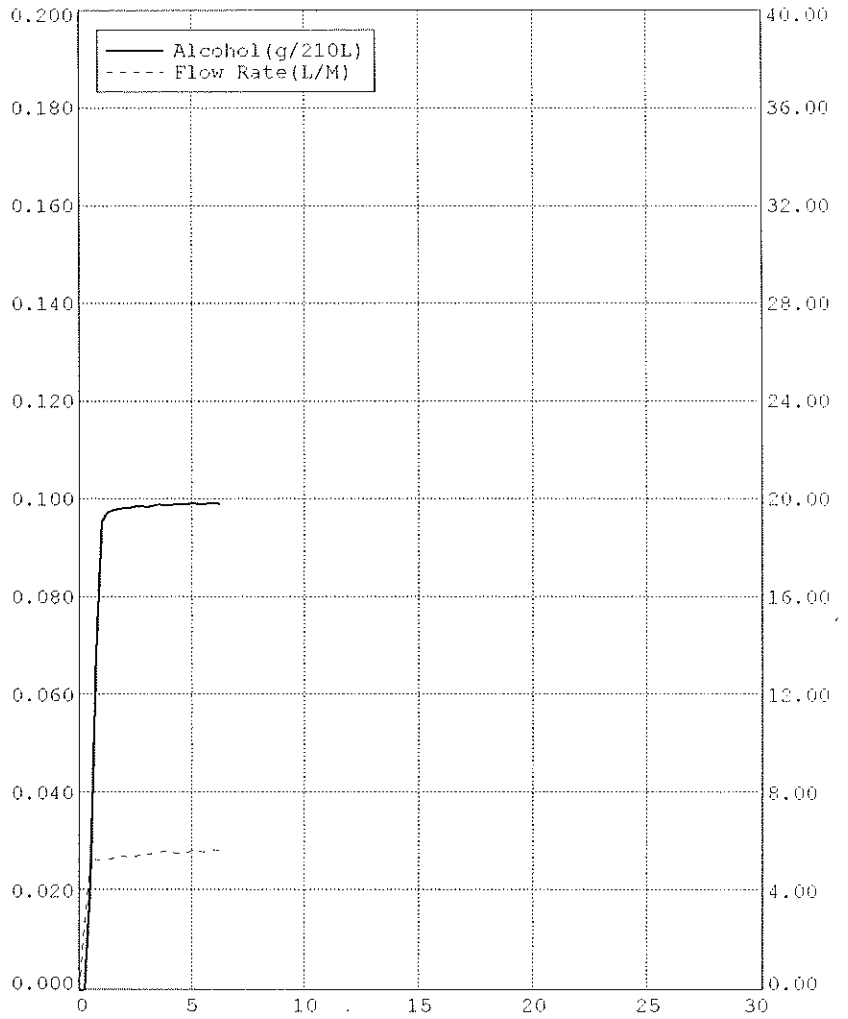



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II
DYLON WYATT

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 3/3/2020

NUMBER 200122

EXPIRES 3/3/2022

MO 580-0771 (6-10)

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

LAB-4 (R6-10)

 STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator WYATT, DYLAN
 Permit No 200122
 Date Issued 3/3/2020 Date Expires 3/3/2022

