

RECEIVED

By Tracy Crews at 3:33 pm, Dec 04, 2020



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500187	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 12/03/2020
LOCATION OF INSTRUMENT (STREET AND CITY) Montgomery County Jail, 211 E 3rd., Montgomery City		TIME OF INSPECTION 17:41:54

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

 DIAGNOSTIC RECORD

DATE AND TIME <u>12/03/2020 17:41:56</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.8°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG011501</u> EXP. DATE <u>04/24/2022</u>
<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

- 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.100	TEST 2: 0.100	TEST 3: 0.100
---------------	---------------	---------------

 PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 0	OVER .19: 1
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

Maintenance Check After Internal Standard Change

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME RAYMOND S MILLER	
TYPE II PERMIT NUMBER 290269	EXPIRATION DATE 11/07/2021	TELEPHONE NUMBER 573-751-1000

RETURN COMPLETED REPORT TO THE
Breath Alcohol Program, Missouri Department of Health and Senior Services
by mail, fax, or email

STANDARD CHANGE

Missouri State Highway Patrol
INTOX dmt: 500187

Date: 12/03/2020
Time: 17:26:10

OPERATOR NAME:
RAYMOND S MILLER
PERMIT NUMBER: 290269
EXPIRATION DATE: 11/07/2021


LOT #: AG011501
SUPPLIER: INTOXIMETERS
EXPIRATION: 04/24/2022
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION
CONCENTRATION: 0.100
TARGET: 0.097

BLANK TEST	0.000	17:27
INTERNAL STANDARD	VERIFIED	17:27
EXTERNAL STANDARD	0.098	17:27
BLANK TEST	0.000	17:28

Average = 0.0980
Std Dev = 0.0000
Spread = 0.0000

RS Miller

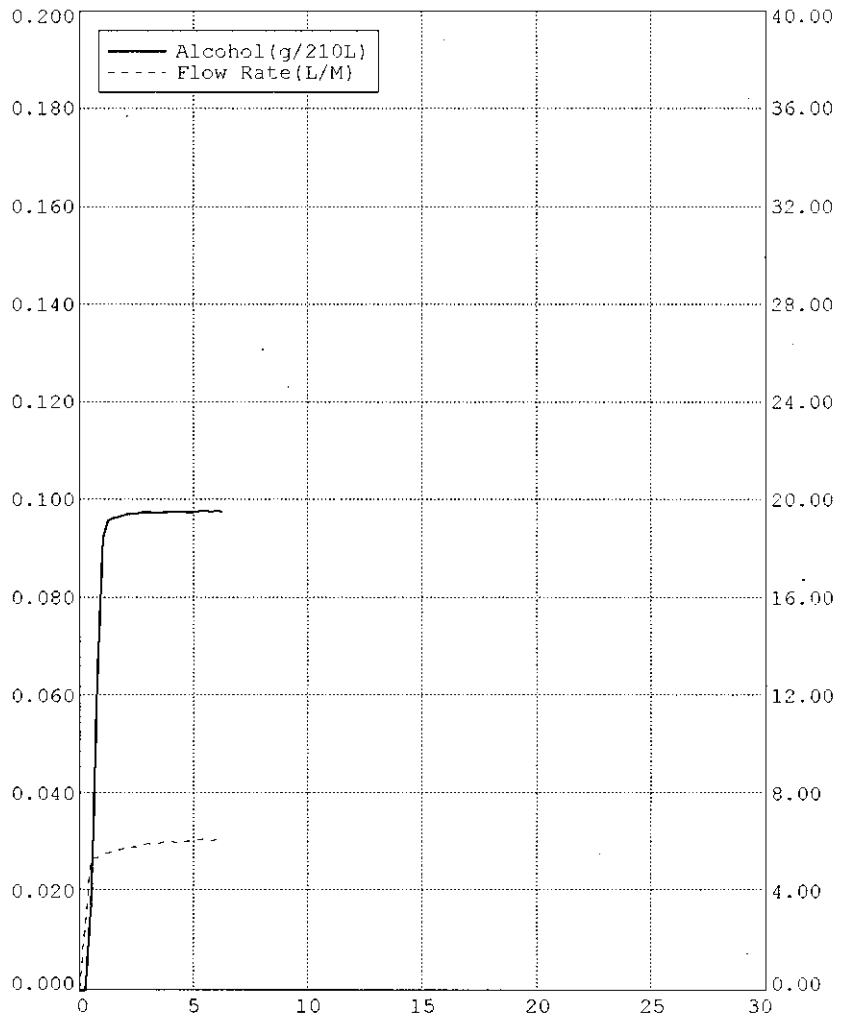



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

2

PERMIT
TYPE II
RAYMOND S MILLER

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX EC/IR II

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 11/7/2019

NUMBER 290269

EXPIRES 11/7/2021

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES

STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator MILLER, RAYMOND
Permit No 290269
Date Issued 11/7/2019 **Date Expires** 11/7/2021