

**RECEIVED**

By Tracy Crews at 10:27 am, Jun 29, 2020

MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
STATE PUBLIC HEALTH LABORATORY  
BREATH ALCOHOL PROGRAM**INTOX DMT MAINTENANCE REPORT**

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).  
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500202	NAME OF AGENCY Missouri State Highway Patrol	DATE OF INSPECTION 06/23/2020
LOCATION OF INSTRUMENT (STREET AND CITY) Reynolds Co. Sheriff's Dept, Centerville, MO		TIME OF INSPECTION 15:36:31

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

 DIAGNOSTIC RECORDDATE AND TIME 06/23/2020 15:36:33 DETECTOR PROGRAM FILTER 1 SAMPLE CHAMBER 48.7°C FILTER 2 BREATH TUBE 44.3°C FILTER 3 PUMP INTERNAL STANDARD

## BREATH ANALYZER ACCURACY STANDARDS

 SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE STANDARD SUPPLIER AIRGAS LOT # AG004403 EXP. DATE 02/13/2022 SIMULATOR TEMP (34°C ± 0.2°C) \_\_\_\_\_ SIMULATOR SN \_\_\_\_\_ SIMULATOR EXP DATE \_\_\_\_\_

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)  
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.100

TEST 2: 0.100

TEST 3: 0.100

 PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0

0-.04: 0

.05-.09: 0

.10-.14: 1

.15-.19: 0

OVER .19: 0

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

June Maintenance

**INSPECTING OFFICER**

SIGNATURE

PRINT FULL NAME

COREY T MORGAN

TYPE II PERMIT NUMBER

290218

EXPIRATION DATE

09/25/2021

TELEPHONE NUMBER

417-469-3121

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services  
Southeast District Office  
2875 James Blvd, Poplar Bluff, MO 63901

STANDARD CHANGE

-----  
Missouri State Highway Patrol  
INTOX dmt: 500202  
-----

Date: 06/23/2020  
Time: 15:33:00


OPERATOR NAME:  
COREY T MORGAN  
PERMIT NUMBER: 290218  
EXPIRATION DATE: 09/25/2021

LOT #: AG004403  
SUPPLIER: AIRGAS  
EXPIRATION: 02/13/2022  
SIMULATOR TYPE: DRY GAS

STANDARD INFORMATION  
CONCENTRATION: 0.100  
TARGET: 0.097

BLANK TEST	0.000	15:33
INTERNAL STANDARD	VERIFIED	15:34
EXTERNAL STANDARD	0.098	15:34
BLANK TEST	0.000	15:35

Average = 0.0980  
Std Dev = 0.0000  
Spread = 0.0000

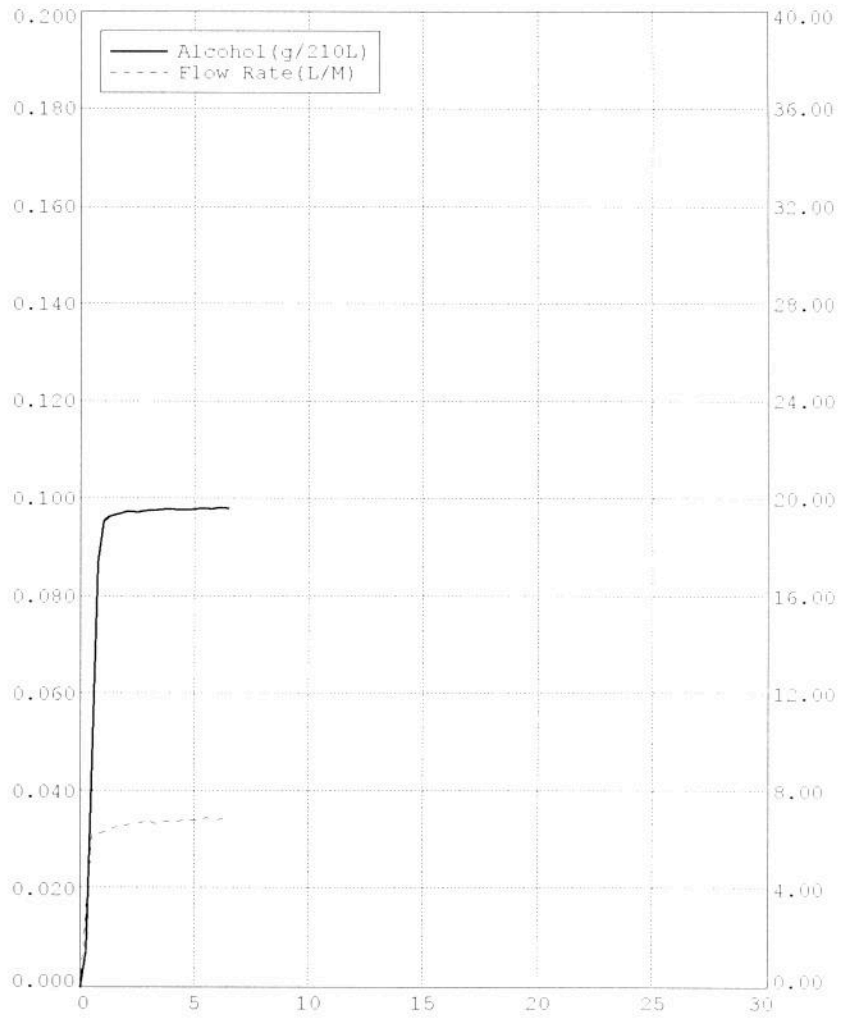



STATE OF MISSOURI  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM



**PERMIT**  
**TYPE II**  
**COREY MORGAN**

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

**INTOX DMT**

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE 9/25/2019

NUMBER 290218

EXPIRES 9/25/2021

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES



**STATE OF MISSOURI**  
 DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 BREATH ALCOHOL PROGRAM

**INSTRUMENT OPERATOR CARD**

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

**Operator** MORGAN, COREY  
**Permit No** 290218  
**Date Issued** 9/25/2019    **Date Expires** 9/25/2021



KEYNOLDS



Airgas USA LLC (LAB)  
3500 Bernard Street  
St. Louis, Mo. 63103  
Ph: (314) 533-3100  
Fax: (314) 533-7328

## Certificate of Analysis

**Customer Name**

Exclusive Supplier  
Intoximeters, Inc.  
2081 Craig Road  
St. Louis, Mo 63146

**Test Date:** 17-Feb-2020

**Lot # AG004403 Model 108cadd**

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
13-Feb-2022	108	Ethanol Nitrogen	0.100 ± 2% BrAC (260 ppm) Balance

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u>	<u>Concentration</u>	<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>	<u>CRM Serial No.</u>	<u>Concentration</u>
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

**Analytical Method:** NDIR

Digitally signed by Quality Control  
Date: 2020.02.18 10:32:01 -06:00  
Reason: Dry gas standard certification of analysis  
Location: Airgas USA LLC (Lab)

Approved for Release: \_\_\_\_\_

*Rod Marsala*  
Rod Marsala

**ISO 17025:2005 A2LA accredited. Certificate Number 3082.06**  
**ISO 17034:2016 A2LA accredited. Certificate Number 3082.07**