



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

RECEIVED
 By Tracy Crews at 8:51 am, Nov 03, 2020

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500222	NAME OF AGENCY Cape Girardeau Police Department	DATE OF INSPECTION 11/02/2020
LOCATION OF INSTRUMENT (STREET AND CITY) 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		TIME OF INSPECTION 08:13:31

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>11/02/2020 08:13:34</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG916501 EXP. DATE 06/14/2021

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIM. SN _____ SIM. NIST EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.081 TEST 2: 0.081 TEST 3: 0.080

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 0	0-.04: 0	.05-.09: 0	.10-.14: 0	.15-.19: 1	OVER .19: 0
-------------	----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

MAINTENANCE

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY
---------------	-------------------------------------

TYPE II PERMIT NUMBER 280323	EXPIRATION DATE 11/19/2020	TELEPHONE NUMBER 573-335-6621
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE
 Breath Alcohol Program, Missouri Department of Health and Senior Services
 by mail, fax, or email



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier

Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 15-Jun-2019

Lot # AG916501 **Model** 108cacd

<u>Exp. Date</u>	<u>Cyl. Type</u>	<u>Component</u>	<u>Certified Concentration</u>
14-Jun-2021	108	Ethanol Nitrogen	0.080 ± 0.002 BrAC (208 ppm) Balance

Certification Traceable to N.I.S.T. RGM and to CRM Ethanol Standards:

<u>RGM Serial No.</u>	<u>Concentration</u>	<u>RGM Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

<u>CRM Serial No.</u>	<u>Concentration</u>	<u>CRM Serial No.</u>	<u>Concentration</u>
CC434668	800.0 ppm	0056649	390.1 ppm
CC234503	253.0 ppm	0056662	150.2 ppm

Analytical Method: NDIR

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 3082.06
ISO 17034:2016 A2LA accredited. Certificate Number 3082.07



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM



PERMIT
TYPE II
JACOB W MARBERRY

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field service and repairs, and operate the following breath analyzer(s):

INTOX DMT

for the determination of the alcoholic content of blood from a sample of expired air. Permit issued under the provisions of sections 577.020 through 577.041, RSMo and 306.111 through 306.119 RSMo.

DATE **11/19/2018**

NUMBER **280323**

EXPIRES **11/19/2020**

DIRECTOR OF STATE PUBLIC HEALTH LABORATORY

DIRECTOR OF DEPARTMENT OF HEALTH AND SENIOR SERVICES



STATE OF MISSOURI
 DEPARTMENT OF HEALTH AND SENIOR SERVICES
 BREATH ALCOHOL PROGRAM

INSTRUMENT OPERATOR CARD

The named cardholder is authorized to operate an evidential breath alcohol instrument for the determination of the alcoholic content in breath form of expired air in Missouri.

Operator MARBERRY, JACOB
Permit No 280323
Date Issued 11/19/2018 **Date Expires** 11/19/2020



RECEIVED

By Tracy Crews at 9:54 am, Nov 19, 2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

APPROVED

By Stephen Wilson at 11:19 am, Nov 19, 2018

APPLICATION FOR TYPE II PERMIT FOR OPERATION OF BREATH ALCOHOL ANALYZERS

THIS APPLICATION IS FOR <input type="checkbox"/> NEW PERMIT <input checked="" type="checkbox"/> RENEWAL		CURRENT PERMIT NUMBER AND EXPIRATION DATE 260341 11-17-2018	
PRINT FULL NAME Jacob W Marberry		TITLE Patrolman	AGE 30
[REDACTED]		A disclosure concerning your SSN number is available at: http://www.health.mo.gov/lab/breathalcohol/	
DEPARTMENT OR TROOP Cape Girardeau MO Police		TELEPHONE (573) 335-6621	
BUSINESS ADDRESS (STREET, CITY, STATE, ZIP CODE) 2530 Maria Louise, Cape Girardeau, MO 63701			
EMAIL ADDRESS jmarberry@cityofcapegirardeau.org			

LIST ALL ORIGINAL TRAINING COURSES FOR OPERATION OF BREATH ANALYZERS
(Also, please place a checkmark beside ALL breath analyzer(s) for which you are requesting a permit.)

DATES OF COURSE	LOCATION OF COURSE	COURSE LENGTH (HRS.)	NAME & MODEL OF BREATH ANALYZER	PLACE A / BESIDE INSTRUMENTS FOR WHICH YOU REQUEST	NAME OF INSTRUCTOR
2010	SEMO LE Academy	40	Datamaster	<input type="checkbox"/>	Eudy
10-2014	UCM/MSC	40	Type II Supervisor (IntoxDMT)	<input checked="" type="checkbox"/>	Welsh
11-2014	UCM/MSC	14	IntoxDMT	<input checked="" type="checkbox"/>	Welsh
				<input type="checkbox"/>	

List the manufacturer and name of instruments for which you are currently performing maintenance reports on and the number of maintenance reports performed on EACH type in the last year.

MANUFACTURER AND NAME OF INSTRUMENT	NUMBER OF MAINTENANCE REPORTS	NUMBER OF SUBJECT TESTS
1. IntoxDMT	2 OK SGW	5 Self Tests OK SGW
2.		
3.		

When adding a new instrument, you receive a new two (2) year permit. Therefore, normal renewal procedures apply for the instrument(s) on your current permit that you wish to transfer to the new permit. Disregarding these renewal procedures will result in a new permit for the new instrument only.

To renew a Type II Permit, the applicant shall have completed two (2) Maintenance Reports and shall have performed at least ten (10) tests on drinking subjects in the past year on each instrument for which renewal is requested. If these conditions are not met, or the permit has expired for more than thirty (30) days, the applicant shall perform two (2) Maintenance Reports and five (5) self-administered tests for each breath analyzer for which renewal is requested. Copies of the Maintenance Reports along with the Operational checklists and printouts for the five (5) self-administered tests shall accompany the application for renewal.

SIGNATURE OF APPLICANT 	DATE 11/18/2018
----------------------------	--------------------

RETURN COMPLETED APPLICATION TO THE: Breath Alcohol Program, Missouri Department of Health and Senior Services
Southeast District Office
2875 James Blvd.
Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		INSTRUMENT SERIAL NUMBER 500222	DATE OF TEST 11/17/2018	TIME OF TEST 04:56:10
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	04:57
INTERNAL STANDARD	VERIFIED	04:57
SUBJECT SAMPLE (Vol=1.93L)	0.000	04:59
BLANK TEST	0.000	05:00

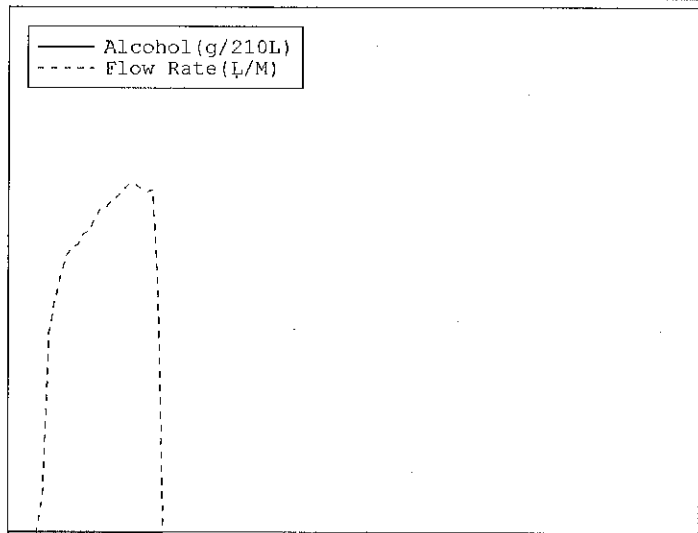

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

J. Marberry

DATE
11/17/2018

WITNESS (IF ANY)

DATE
11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500222	NAME OF AGENCY Cape Girardeau Police Department	DATE OF INSPECTION 10/20/2018
-------------------------------	---	---

LOCATION OF INSTRUMENT (STREET AND CITY) 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO	TIME OF INSPECTION 08:52:17
--	---------------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC RECORD	
DATE AND TIME <u>10/20/2018 08:52:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER 48.7°C	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE 47.0°C	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS	
<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG722402</u>	EXP. DATE <u>08/12/2019</u>
--	------------------------------	------------------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
---	---------------------------	---------------------------------

<input checked="" type="checkbox"/> CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT) Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.	
<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE	
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE	
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE	

TEST 1: 0.079	TEST 2: 0.078	TEST 3: 0.078
----------------------	----------------------	----------------------

<input checked="" type="checkbox"/> PERFORM R.F.I. TEST
--

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 1	0-.04: 13	.05-.09: 3	.10-.14: 2	.15-.19: 5	OVER .19: 2
--------------------	------------------	-------------------	-------------------	-------------------	--------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY
----------------------	---

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
---	---	--

RETURN COMPLETED REPORT TO THE **Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901**



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		INSTRUMENT SERIAL NUMBER 500222	DATE OF TEST 11/17/2018	TIME OF TEST 05:02:14
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	05:03
INTERNAL STANDARD	VERIFIED	05:03
SUBJECT SAMPLE (Vol=1.68L)	0.000	05:03
BLANK TEST	0.000	05:04

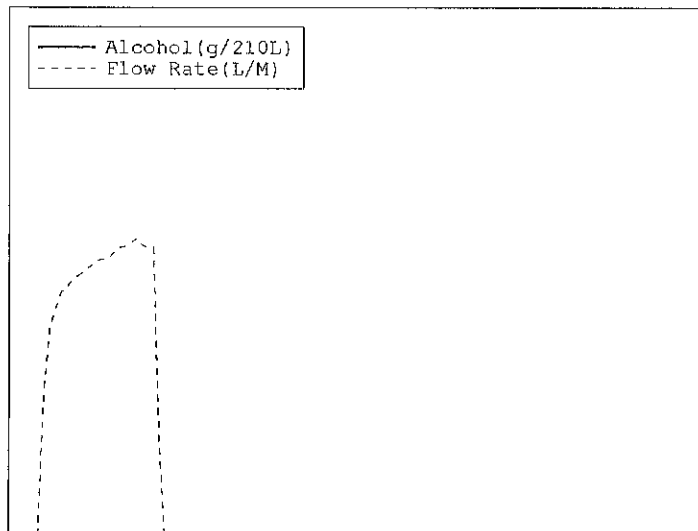

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

J. Marberry

DATE
11/17/2018

WITNESS (IF ANY)

DATE
11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500222	NAME OF AGENCY Cape Girardeau Police Department	DATE OF INSPECTION 10/20/2018
------------------------	--	----------------------------------

LOCATION OF INSTRUMENT (STREET AND CITY) 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO	TIME OF INSPECTION 08:52:17
---	--------------------------------

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>10/20/2018 08:52:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

<input type="checkbox"/> SIMULATOR STANDARD	<input checked="" type="checkbox"/> COMPRESSED ETHANOL-GAS MIXTURE
---	--

<input checked="" type="checkbox"/> STANDARD SUPPLIER <u>INTOXIMETERS</u>	LOT # <u>AG722402</u>	EXP. DATE <u>08/12/2019</u>
---	-----------------------	-----------------------------

<input type="checkbox"/> SIMULATOR TEMP (34°C ± 0.2°C) _____	SIMULATOR SN _____	SIMULATOR EXP DATE _____
--	--------------------	--------------------------

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

<input type="checkbox"/> 0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input checked="" type="checkbox"/> 0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.079	TEST 2: 0.078	TEST 3: 0.078
---------------	---------------	---------------

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 1	0-.04: 13	.05-.09: 3	.10-.14: 2	.15-.19: 5	OVER .19: 2
-------------	-----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY
---------------	-------------------------------------

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
---------------------------------	-------------------------------	----------------------------------

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		INSTRUMENT SERIAL NUMBER 500222	DATE OF TEST 11/17/2018	TIME OF TEST 05:06:15
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	05:07
INTERNAL STANDARD	VERIFIED	05:07
SUBJECT SAMPLE (Vol=1.81L)	0.000	05:08
BLANK TEST	0.000	05:09

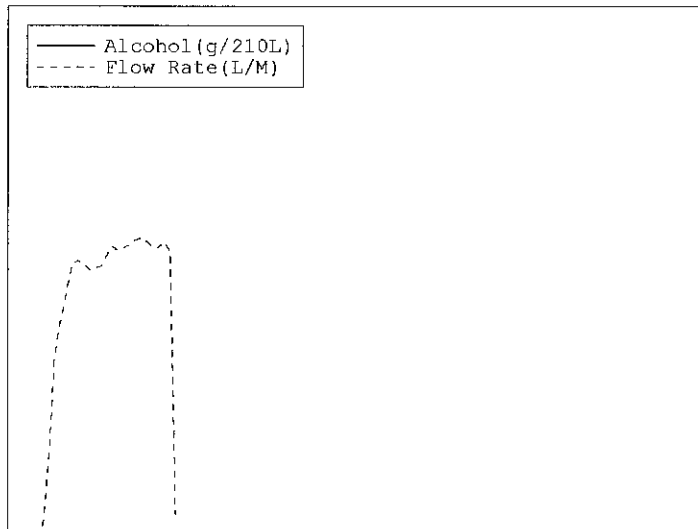

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR

Jacob Marberry

DATE
11/17/2018

WITNESS (IF ANY)

DATE
11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500222	NAME OF AGENCY Cape Girardeau Police Department	DATE OF INSPECTION 10/20/2018
LOCATION OF INSTRUMENT (STREET AND CITY) 2530 MARIA LOUISE LANE CAPE GIRARDEAU, MO		TIME OF INSPECTION 08:52:17

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>10/20/2018 08:52:19</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>47.0°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG722402 EXP. DATE 08/12/2019

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.079 TEST 2: 0.078 TEST 3: 0.078

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: 1	0-.04: 13	.05-.09: 3	.10-.14: 2	.15-.19: 5	OVER .19: 2
-------------	-----------	------------	------------	------------	-------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY	
TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 Maria Louise Ln.		INSTRUMENT SERIAL NUMBER 500223	DATE OF TEST 11/17/2018	TIME OF TEST 04:58:38
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	04:59
INTERNAL STANDARD	VERIFIED	04:59
SUBJECT SAMPLE (Vol=1.79L)	0.000	05:00
BLANK TEST	0.000	05:01

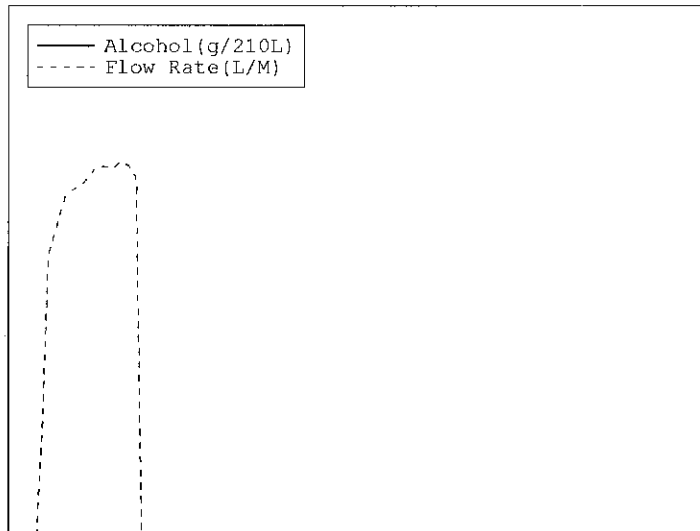

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR 	DATE 11/17/2018
WITNESS (IF ANY)	DATE 11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
STATE PUBLIC HEALTH LABORATORY
BREATH ALCOHOL PROGRAM

INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500223	NAME OF AGENCY Cape Girardeau PD	DATE OF INSPECTION 10/20/2018
LOCATION OF INSTRUMENT (STREET AND CITY) 2530 Maria Louise Ln.		TIME OF INSPECTION 04:30:00

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>10/20/2018 04:30:02</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG805701 EXP. DATE 02/26/2020

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.076 TEST 2: 0.077 TEST 3: 0.076

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: <u>2</u>	<u>0</u> - <u>04</u> : <u>98</u>	<u>05</u> - <u>09</u> : <u>0</u>	<u>10</u> - <u>14</u> : <u>0</u>	<u>15</u> - <u>19</u> : <u>0</u>	OVER <u>19</u> : <u>0</u>
--------------------	----------------------------------	----------------------------------	----------------------------------	----------------------------------	---------------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE 	PRINT FULL NAME JACOB W MARBERRY
---------------	--

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
Southeast District Office
2875 James Blvd, Poplar Bluff, MO 63901



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
BLOOD ALCOHOL TEST REPORT - INTOX DMT

FORM #11


LOCATION OF INSTRUMENT 2530 Maria Louise Ln.		INSTRUMENT SERIAL NUMBER 500223	DATE OF TEST 11/17/2018	TIME OF TEST 05:03:29
SUBJECT NAME JACOB WILLIAM MARBERRY			DATE OF BIRTH 05/01/1988	
SEX M	SUBJECT DRIVER'S LICENSE NUMBER S087121025		STATE MO	
ARRESTING OFFICER JACOB W MARBERRY		ARRESTING OFFICER ID 345		
OPERATOR JACOB MARBERRY		OPERATOR PERMIT 260341	PERMIT EXP DATE 11/17/2018	

OPERATIONAL CHECKLIST: INTOX DMT

- 1. Examination of mouth conducted. If any substance is observed or indicated to be present, the substance observed or indicated must be removed prior to starting the 15 minute observation period.
- 2. Subject observed for at least 15 minutes by JACOB MARBERRY. No smoking, oral intake or vomiting during this time; if vomiting occurs, start over with the 15 minute observation period.
- 3. Assure that the power switch is ON and the screen is displaying "Ready <Push Run>".
- 4. Press the Run button on the display screen.
- 5. Enter subject and officer information.
- 6. When display reads "Please Blow" and gives audible beep, insert mouthpiece and take the subject's breath sample.

SUBJECT TEST RESULTS

BLANK TEST	0.000	05:04
INTERNAL STANDARD	VERIFIED	05:04
SUBJECT SAMPLE (Vol=1.69L)	0.000	05:04
BLANK TEST	0.000	05:05

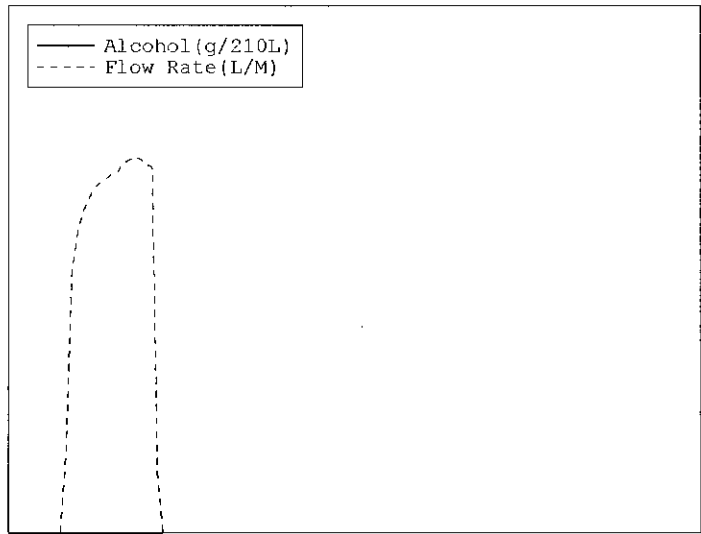

COMMENTS

CERTIFICATION BY OPERATOR

BAC
0.000

As set forth in the rules promulgated by the Department of Health and Senior Services related to the determination of blood alcohol by breath analysis, I certify that:

- 1. There was no deviation from the procedure approved by the department.
- 2. To the best of my knowledge the instrument was functioning properly.
- 3. I am authorized to operate the instrument.
- 4. No radio transmission occurred inside the room where and when this test was being conducted.

SIGNATURE OF OPERATOR <i>Jacob W Marberry</i>	DATE 11/17/2018
WITNESS (IF ANY)	DATE 11/17/2018



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES
 STATE PUBLIC HEALTH LABORATORY
 BREATH ALCOHOL PROGRAM
INTOX DMT MAINTENANCE REPORT

REPORT #1

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 35 days).
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

INTOX DMT SN 500223	NAME OF AGENCY Cape Girardeau PD	DATE OF INSPECTION 10/20/2018
LOCATION OF INSTRUMENT (STREET AND CITY) 2530 Maria Louise Ln.		TIME OF INSPECTION 04:30:00

CHECKLIST: Place a mark in the box by each item if found to be satisfactory or is operating within established limits. (Write in observed values where determined). Unmarked items must be corrected before using instrument.

DIAGNOSTIC RECORD

DATE AND TIME <u>10/20/2018 04:30:02</u>	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTER 1
<input checked="" type="checkbox"/> SAMPLE CHAMBER <u>48.7°C</u>	<input checked="" type="checkbox"/> FILTER 2
<input checked="" type="checkbox"/> BREATH TUBE <u>48.1°C</u>	<input checked="" type="checkbox"/> FILTER 3
<input checked="" type="checkbox"/> PUMP	<input checked="" type="checkbox"/> INTERNAL STANDARD

BREATH ANALYZER ACCURACY STANDARDS

SIMULATOR STANDARD COMPRESSED ETHANOL-GAS MIXTURE

STANDARD SUPPLIER INTOXIMETERS LOT # AG805701 EXP. DATE 02/26/2020

SIMULATOR TEMP (34°C ± 0.2°C) _____ SIMULATOR SN _____ SIMULATOR EXP DATE _____

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)
 Run three tests using a standard. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard being used.

0.10% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE

0.08% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE

0.04% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1: 0.076 TEST 2: 0.077 TEST 3: 0.076

PERFORM R.F.I. TEST

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:

REFUSALS: <u>2</u>	0-04: <u>98</u>	.05-.09: <u>0</u>	.10-.14: <u>0</u>	.15-.19: <u>0</u>	OVER .19: <u>0</u>
--------------------	-----------------	-------------------	-------------------	-------------------	--------------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY)

INSPECTING OFFICER

SIGNATURE <i>JW 345</i>	PRINT FULL NAME JACOB W MARBERRY
----------------------------	--

TYPE II PERMIT NUMBER 260341	EXPIRATION DATE 11/17/2018	TELEPHONE NUMBER 573-335-6621
--	--------------------------------------	---

RETURN COMPLETED REPORT TO THE Breath Alcohol Program, MO Department of Health and Senior Services
 Southeast District Office
 2875 James Blvd, Poplar Bluff, MO 63901



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 14-Aug-2017

Lot # AG722402 **Model** 108cacd

Exp. Date

12-Aug-2019

Cyl. Type

108

Component

Ethanol
Nitrogen

Certified Concentration

0.080 ± 0.002 BrAC (208 ppm)
Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

Analytical Method:

NDIR

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01



Airgas USA LLC (LAB)

3500 Bernard Street

St. Louis, Mo. 63103

Ph: (314) 533-3100

Fax: (314) 533-7328

Certificate of Analysis

Customer Name

Exclusive Supplier
Intoximeters, Inc.
2081 Craig Road
St. Louis, Mo 63146

Test Date: 26-Feb-2018

Lot # AG805701 **Model** 108cacd

Exp. Date

26-Feb-2020

Cyl. Type

108

Component

Ethanol
Nitrogen

Certified Concentration

0.080 ± 0.002 BrAC (208 ppm)
Balance

Certification Traceable to N.I.S.T. RGM Ethanol Standards:

<u>Serial No.</u>	<u>Concentration</u>	<u>Serial No.</u>	<u>Concentration</u>
EB0010581	392.1 ppm	EB0010603	393.0 ppm
EB0010570	259.8 ppm	EB0010559	258.2 ppm
EB0010285	208.0 ppm	EB0010595	208.3 ppm
EB0010561	103.6 ppm	EB0010562	104.2 ppm
EB0010681	52.12 ppm	EB0010579	52.81 ppm

Analytical Method:

NDIR

Approved for Release:

Rod Marsala

ISO 17025:2005 A2LA accredited. Certificate Number 2989.01